


Fig. 1

2022FO" 6904500T

1/32

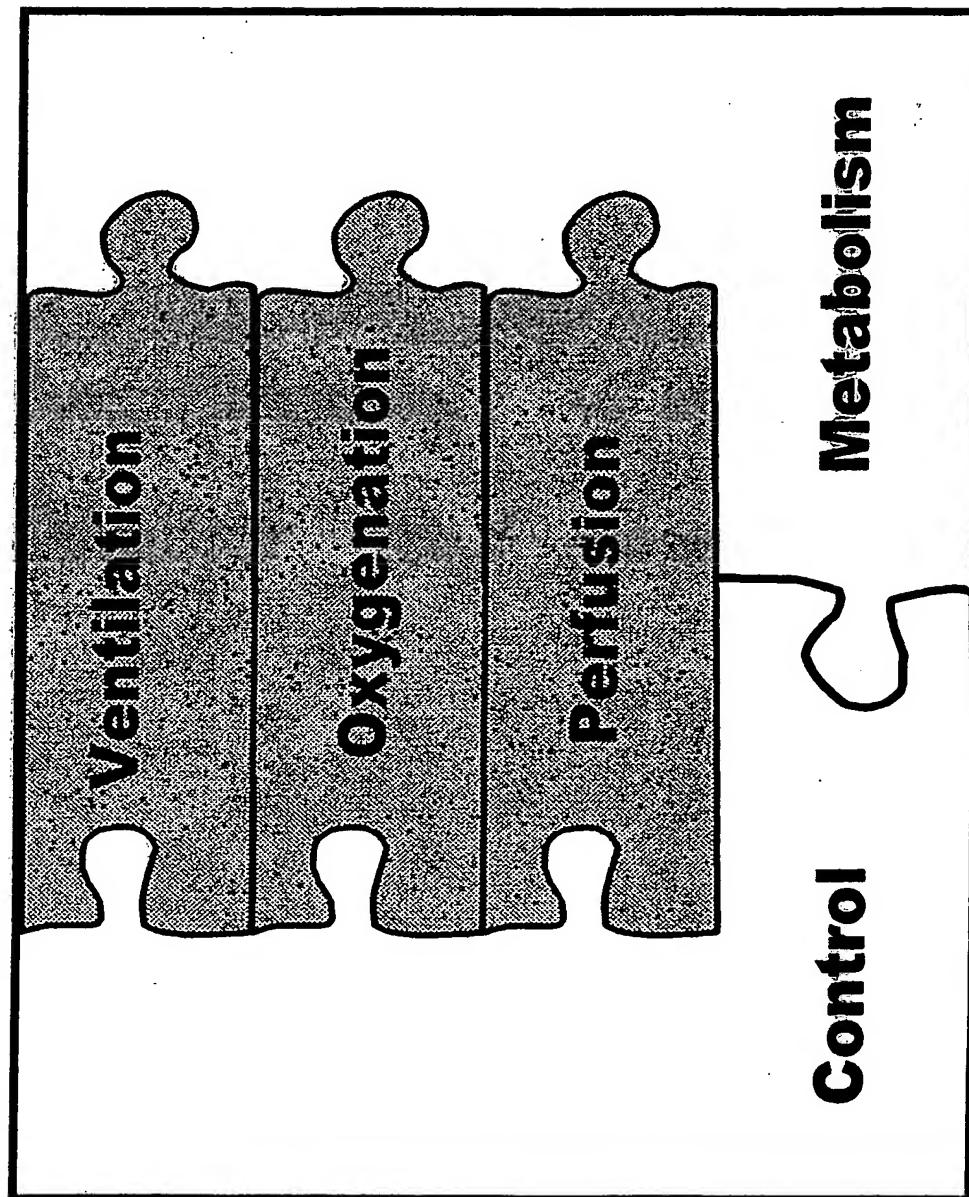

2 →

Figure 2

2022FO 69045001

Extended Heart Object


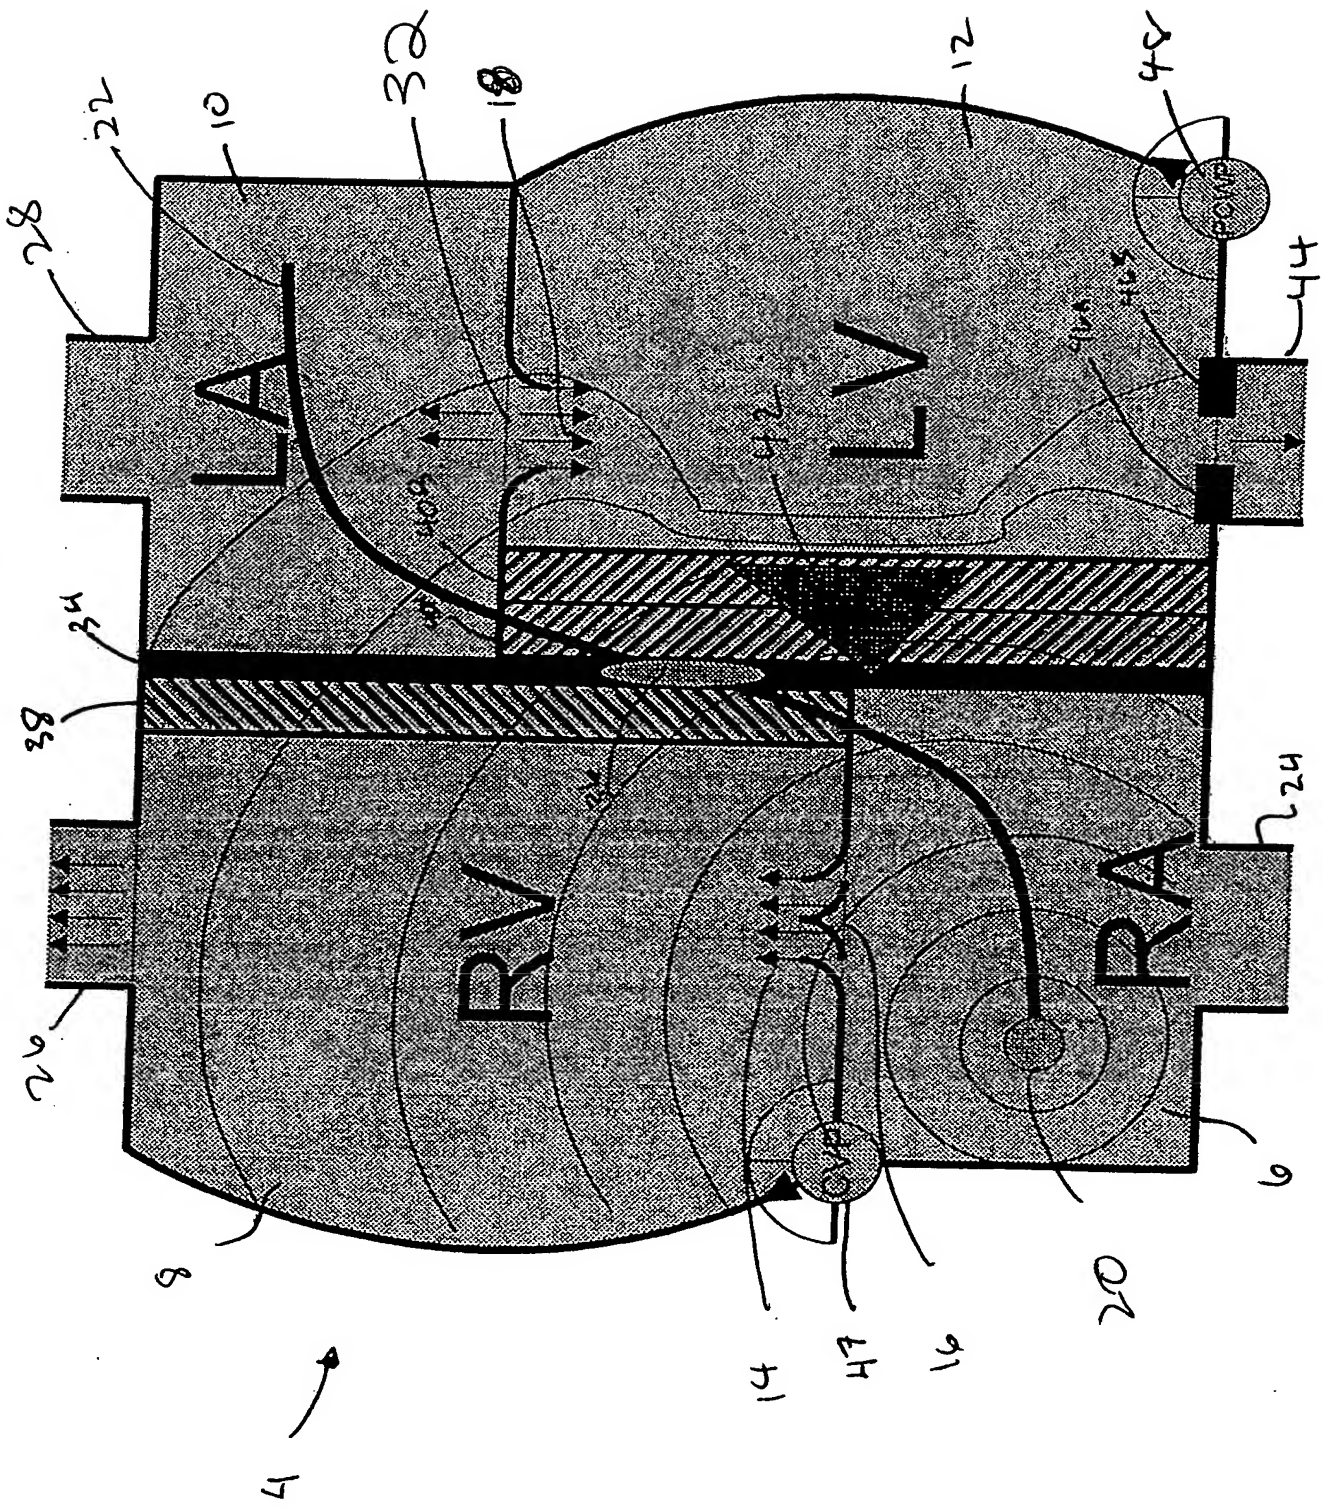



Figure 3


2025-06-01 20:22

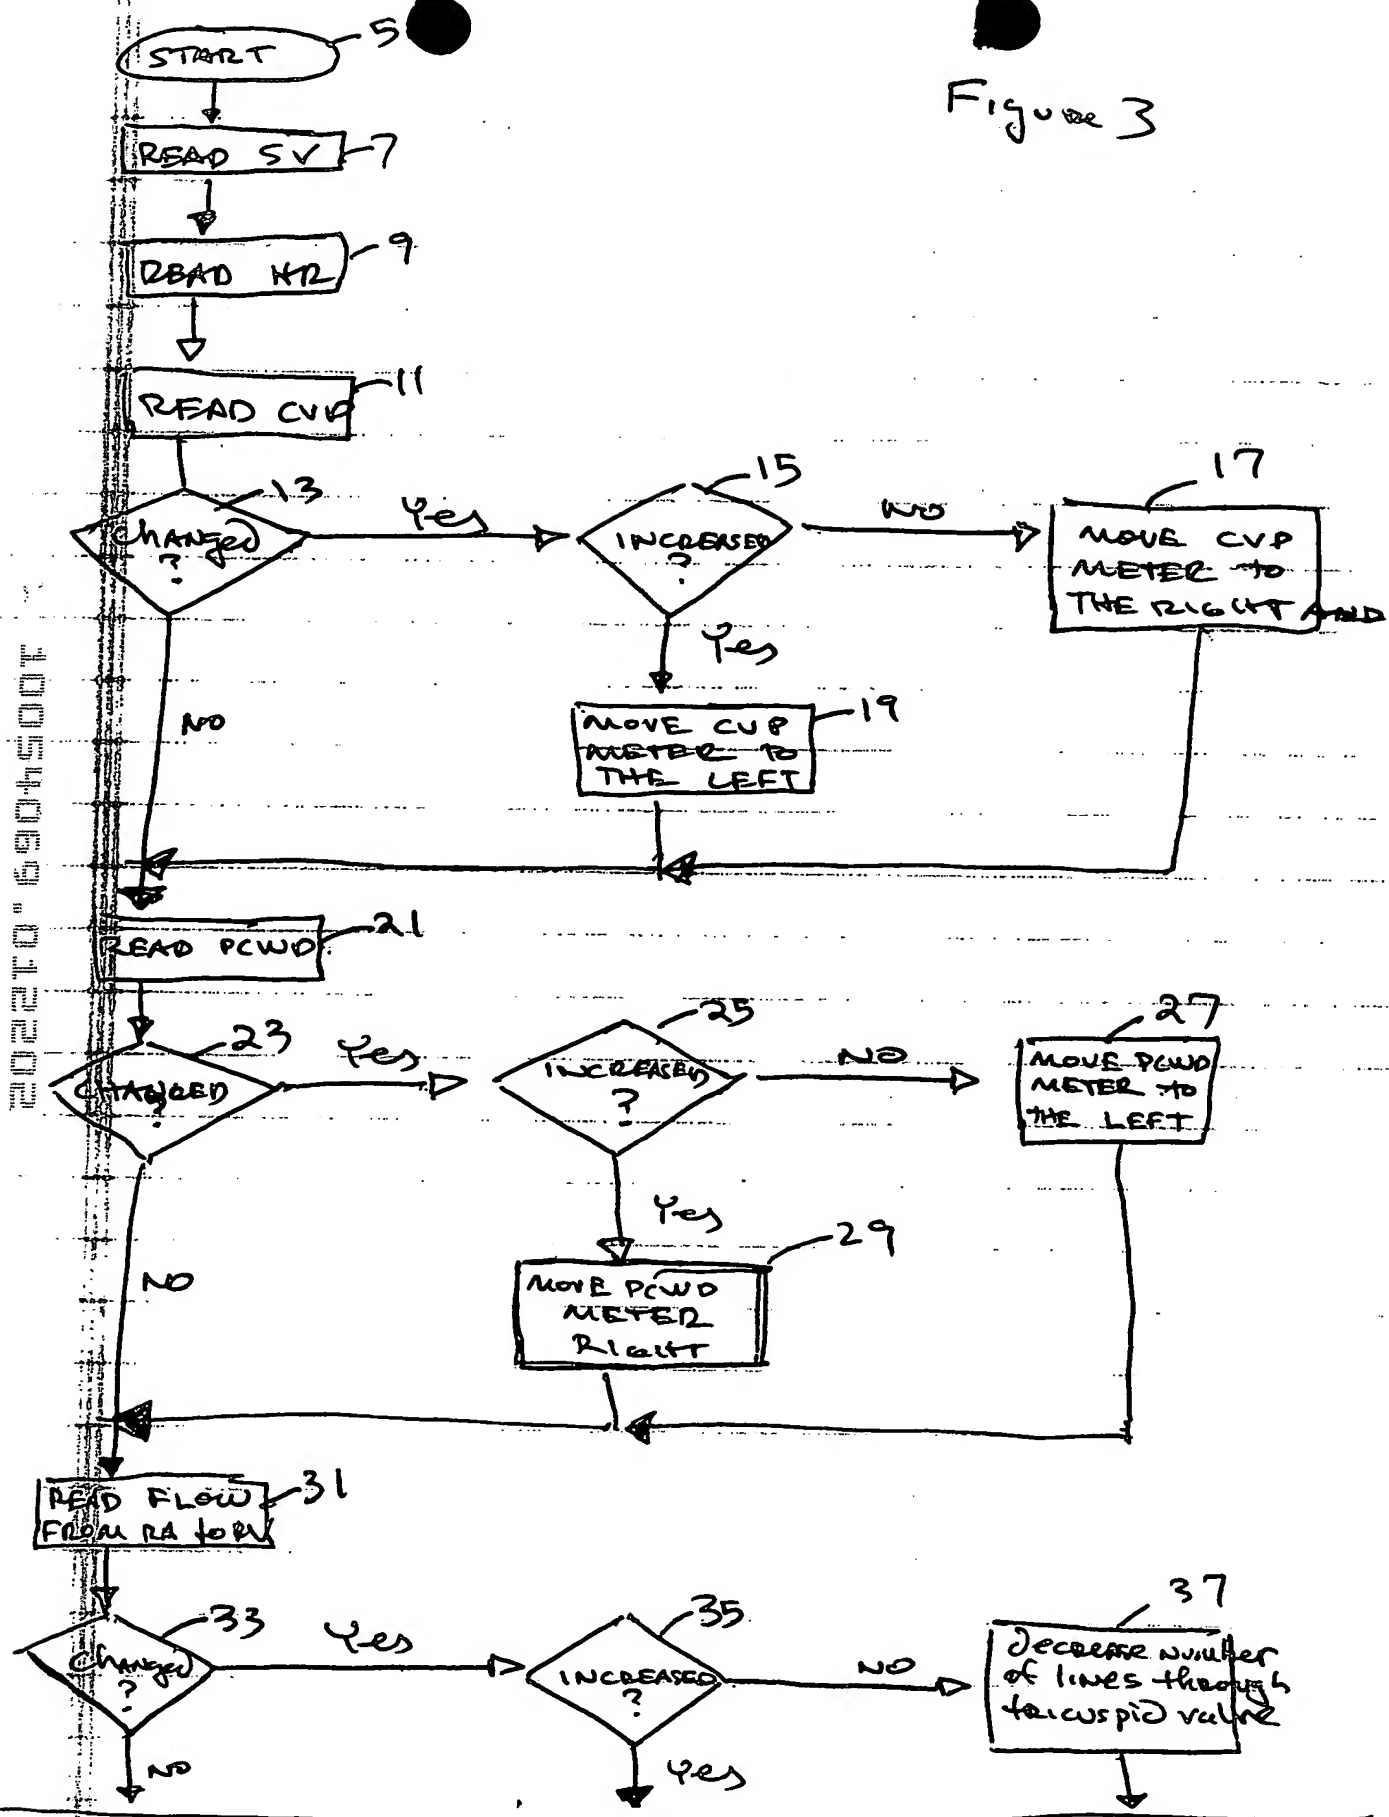


4/32

2022106901202

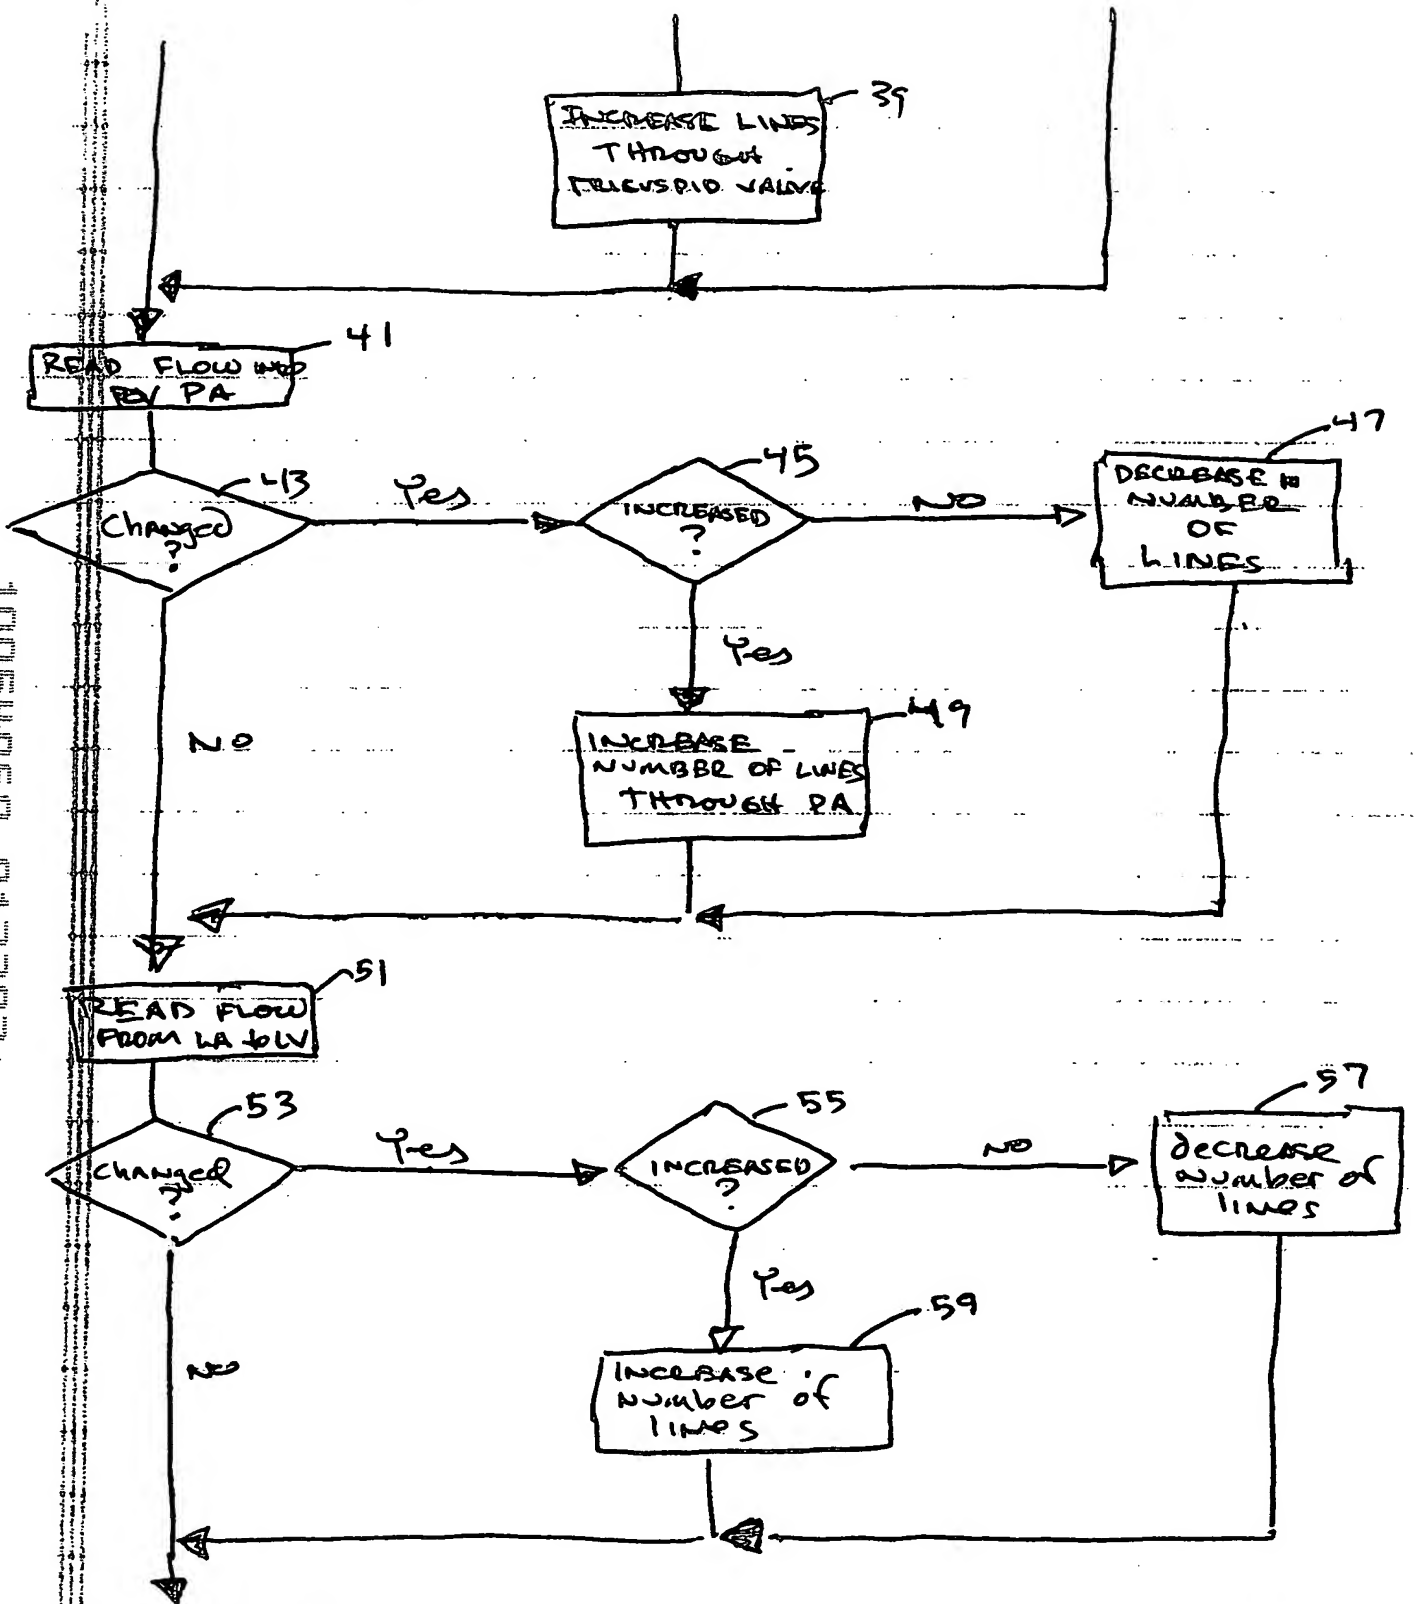

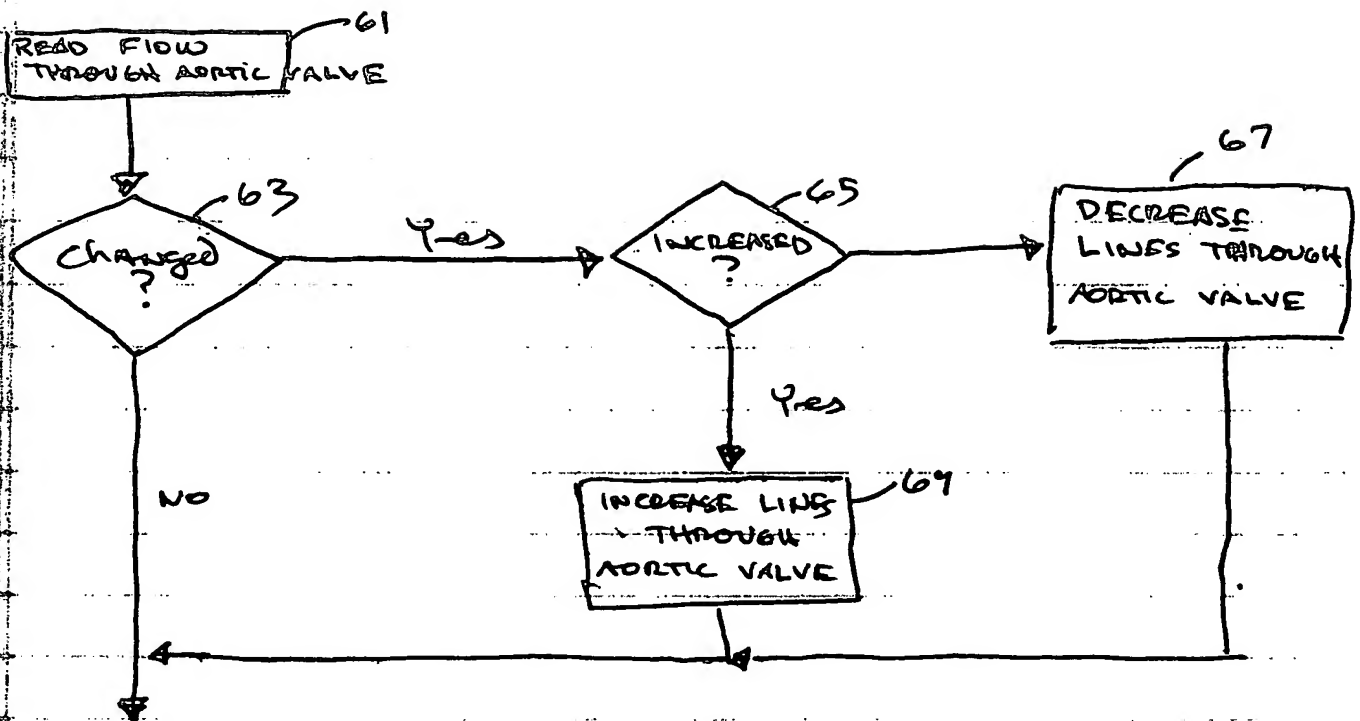


(INSERT TRIANGLE INFORMATION)
71-79

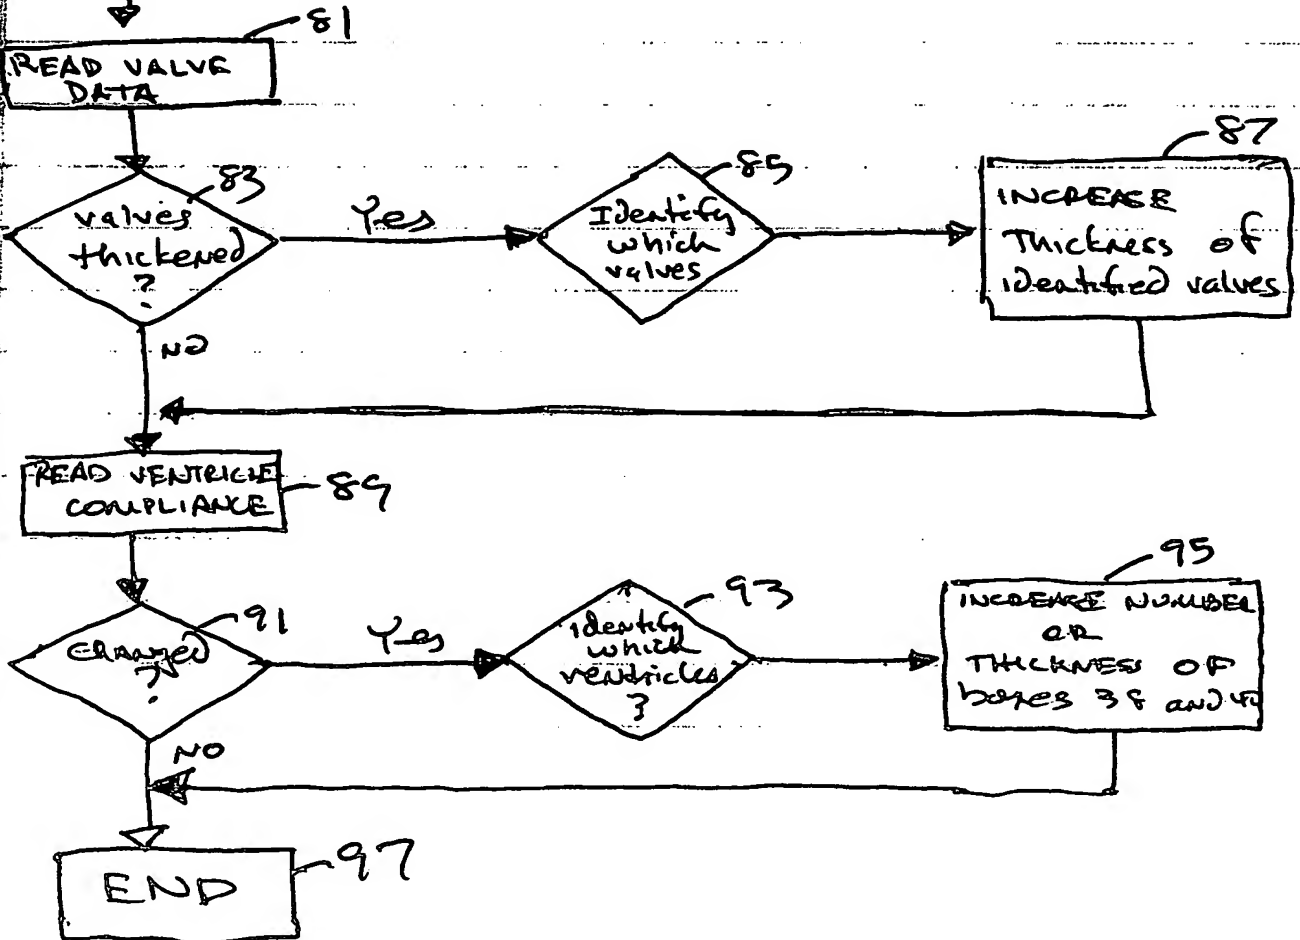

10054069 012202

Fig. 4

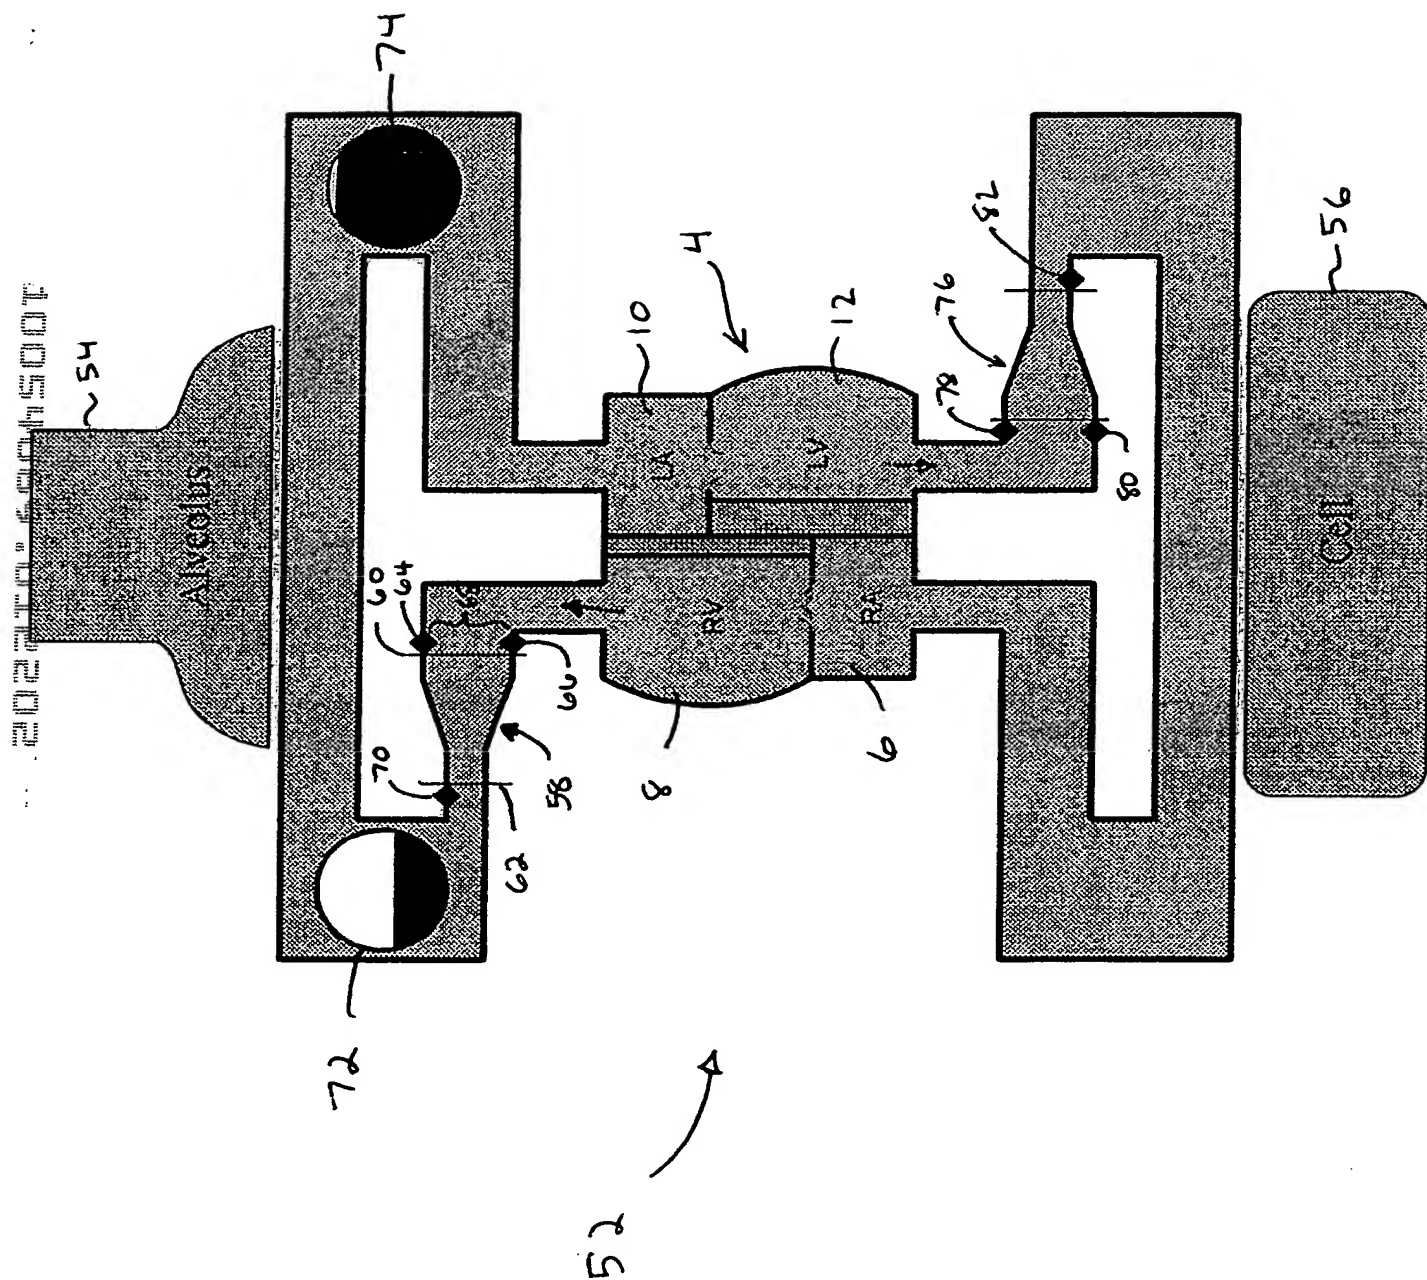

Vascular Circuit (split RV and LV version)


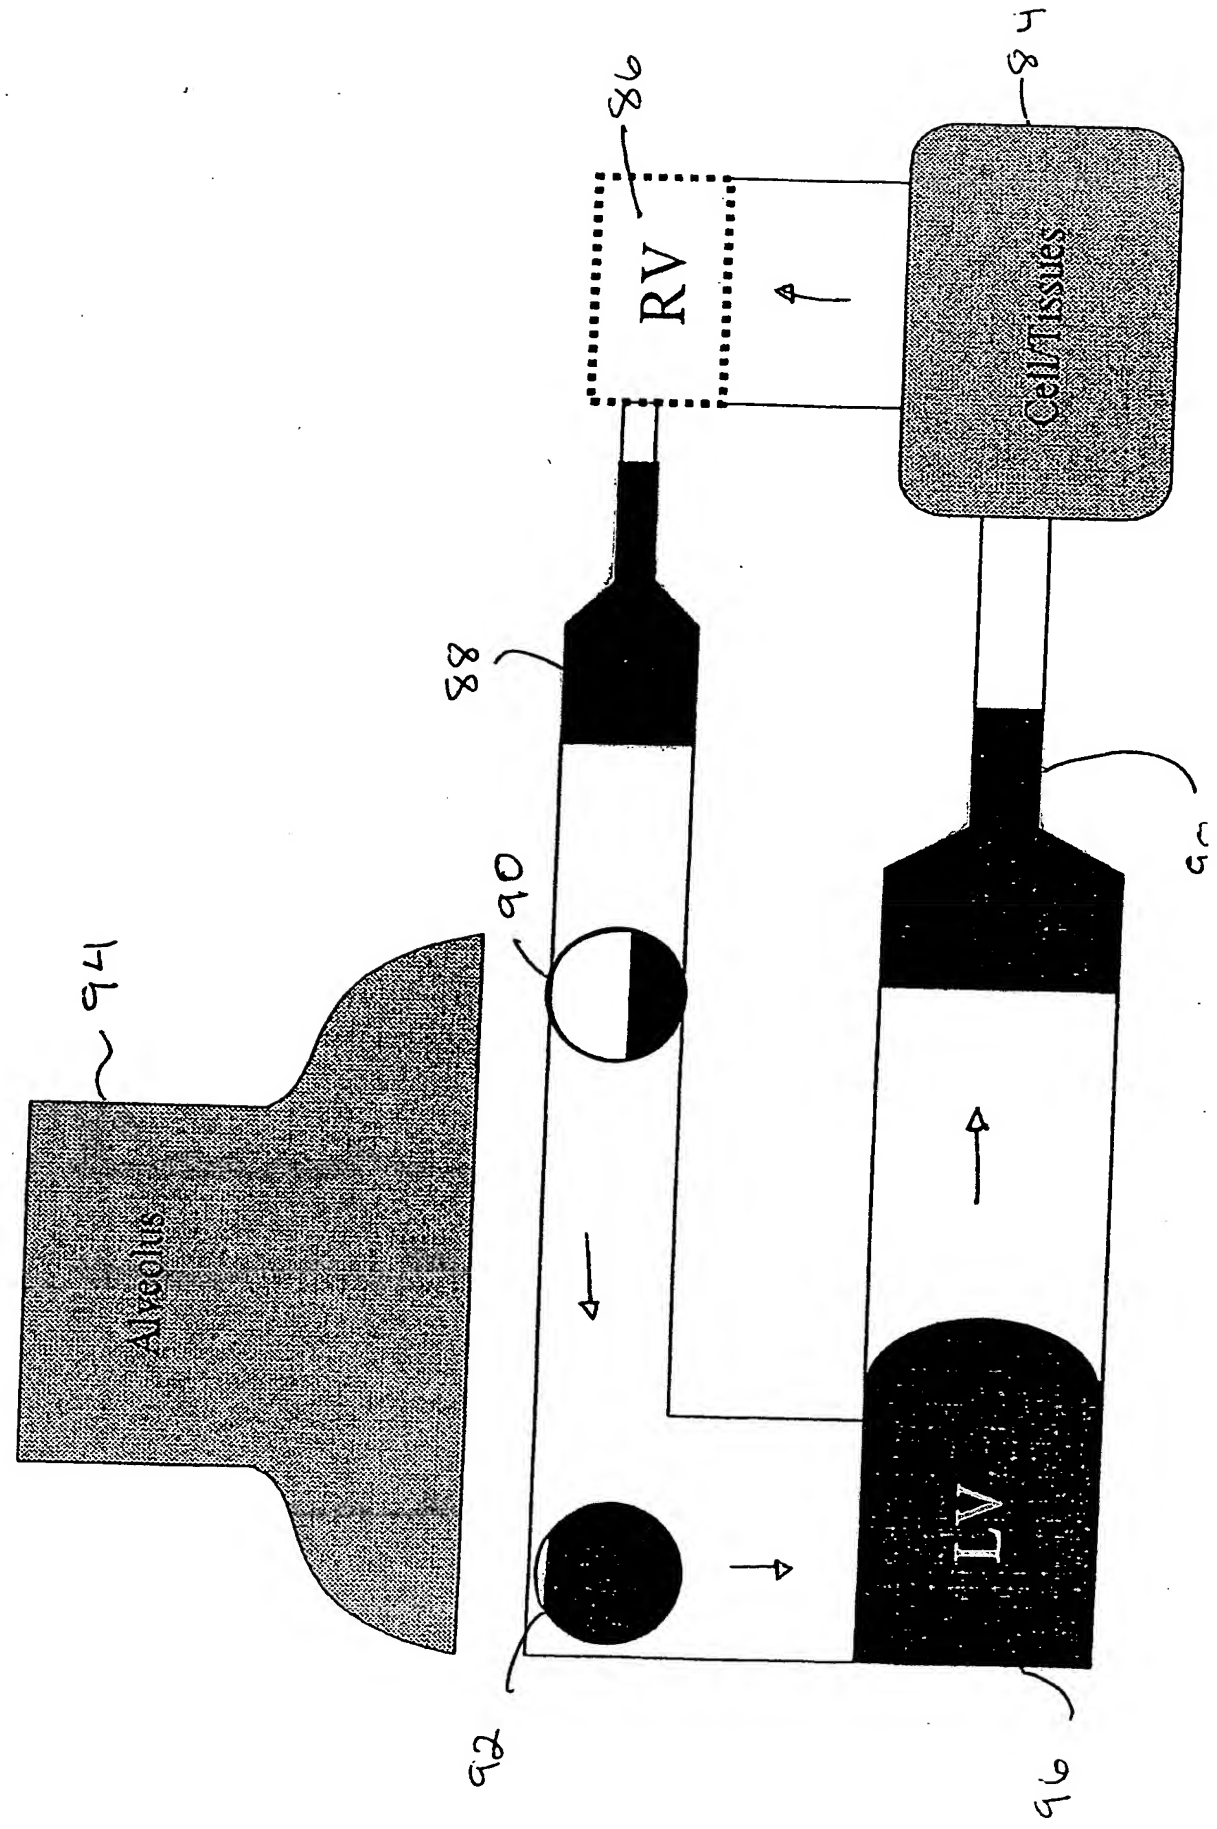


Fig. 6

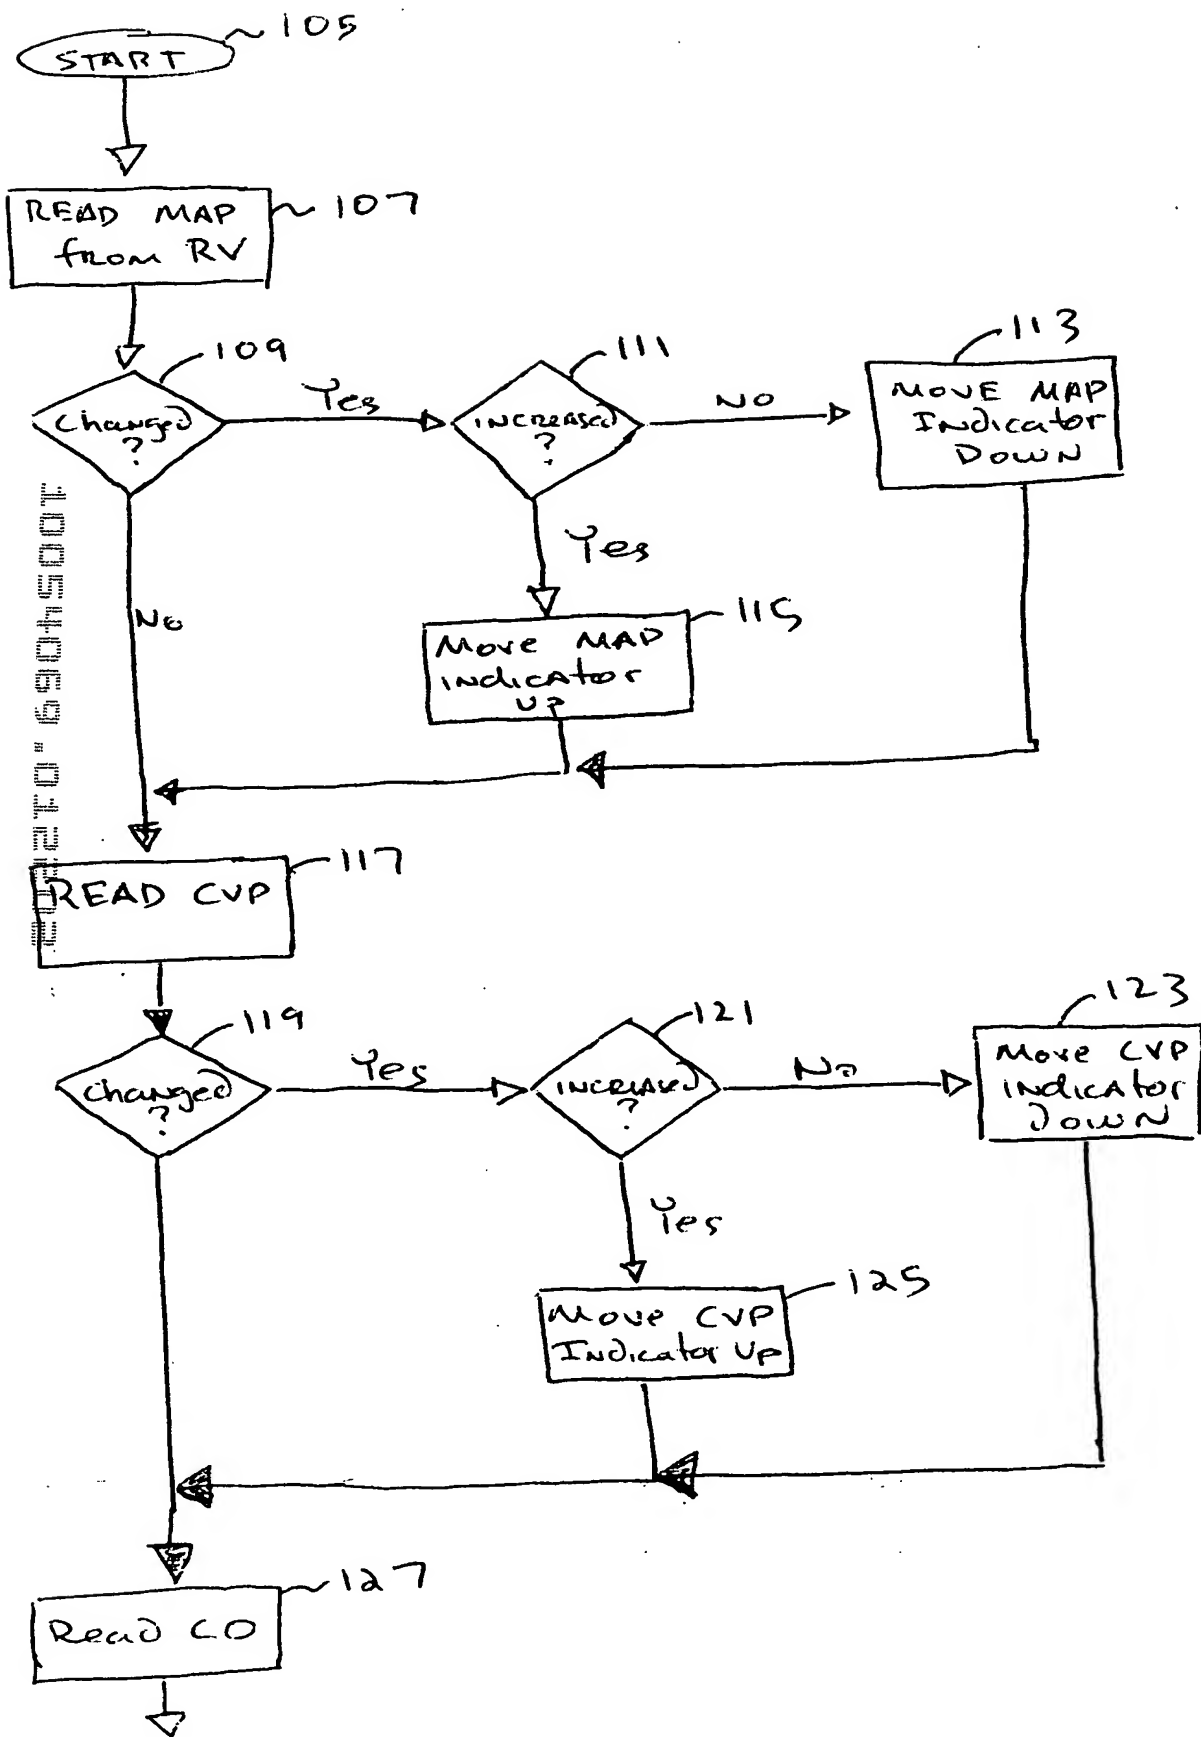

9/32

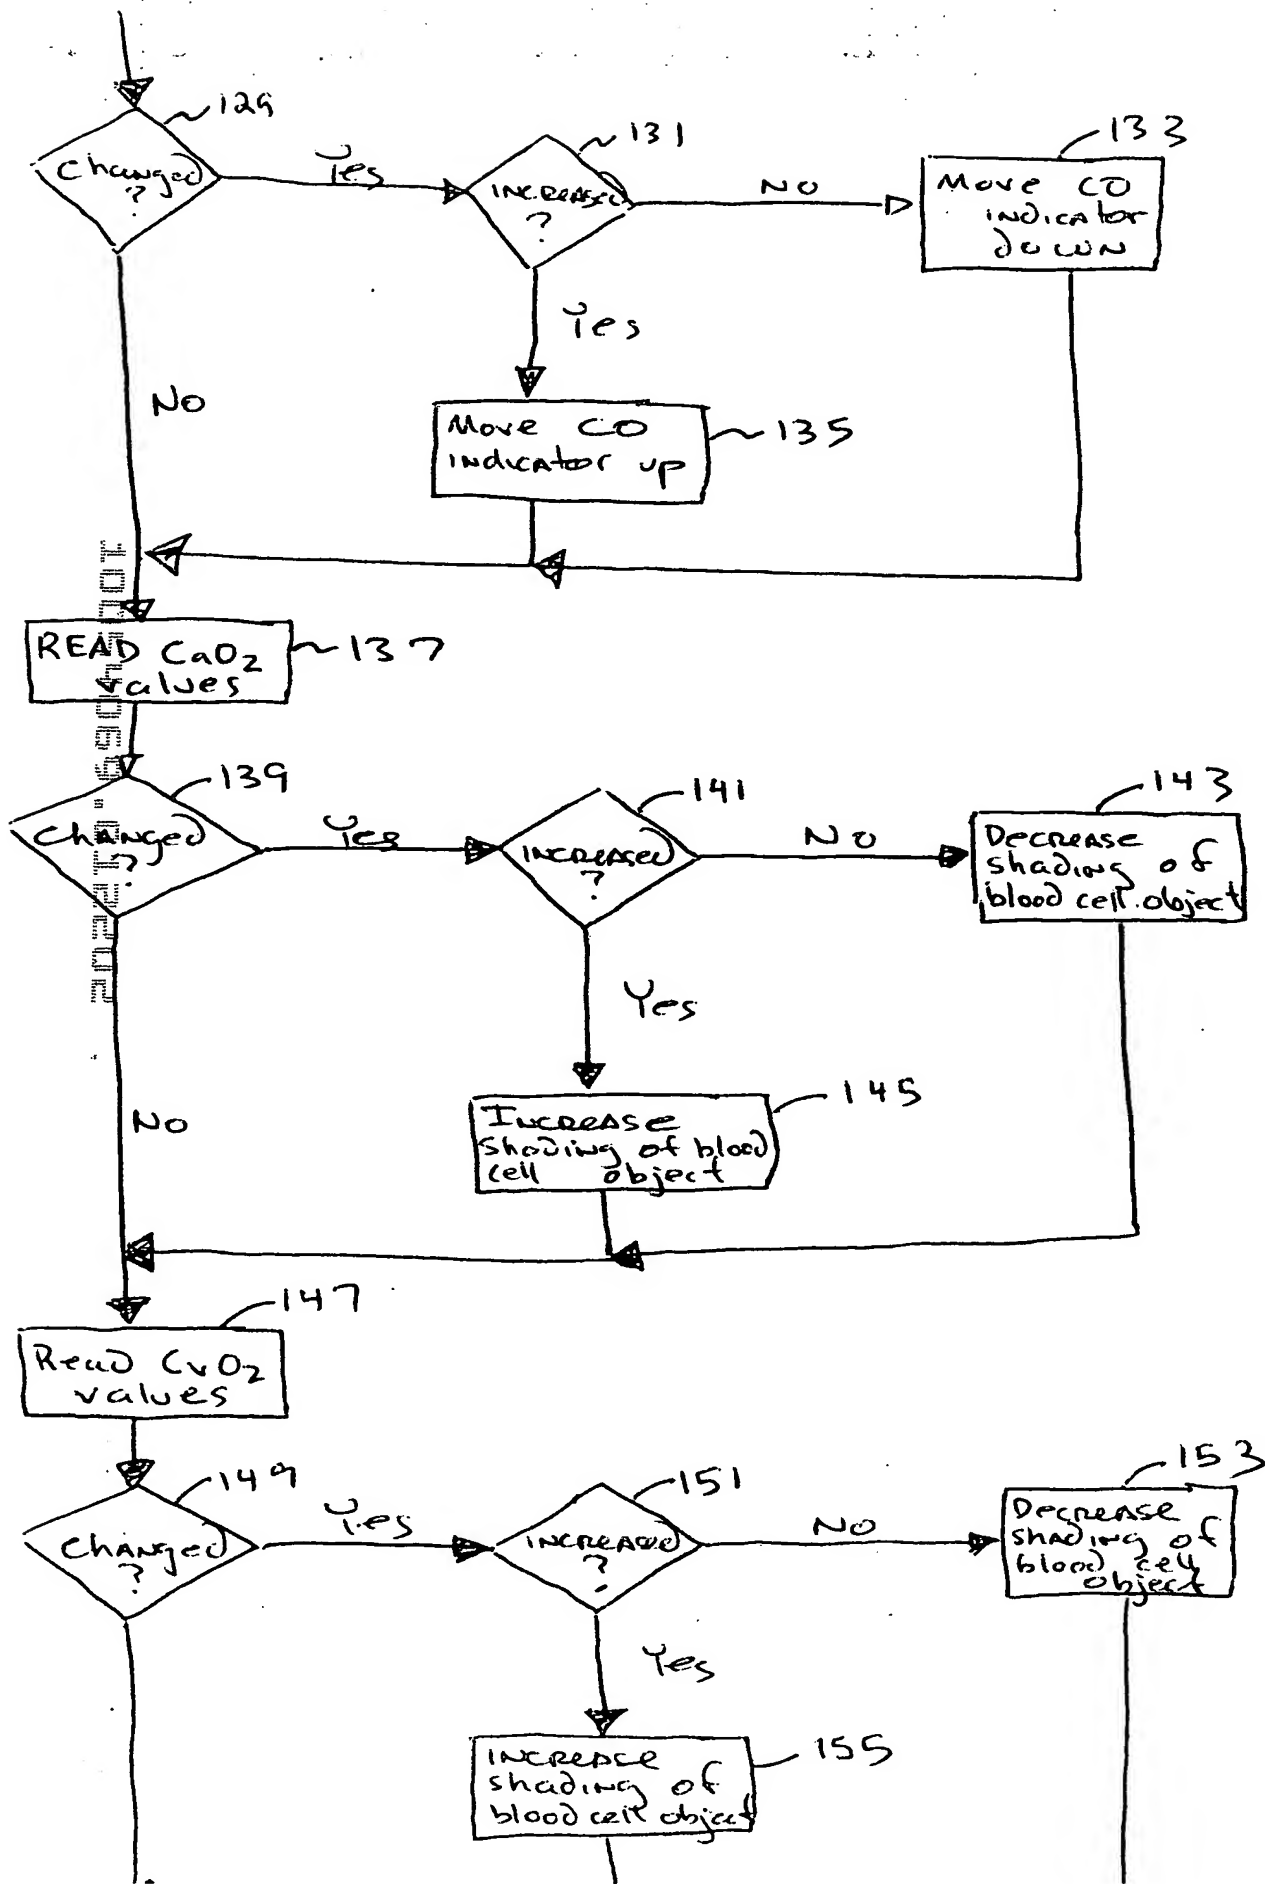


Fig. 7

Cardiopulmonary Bypass Object

2022FO*6904500T

10/32

102

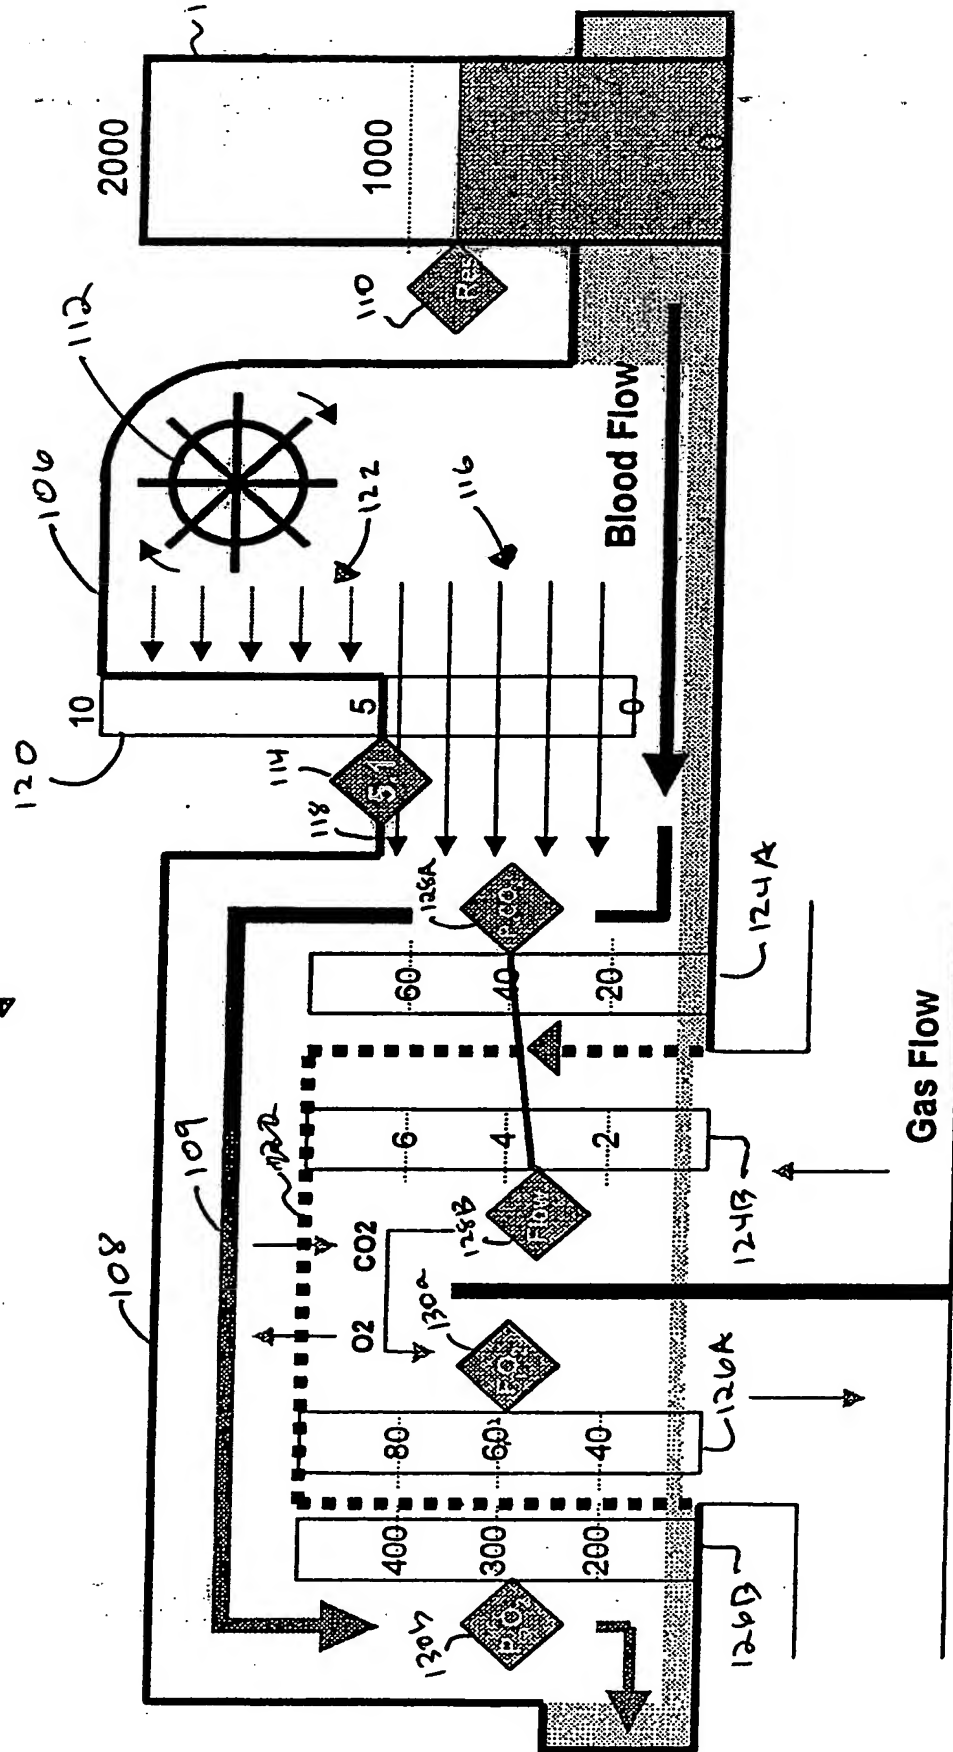
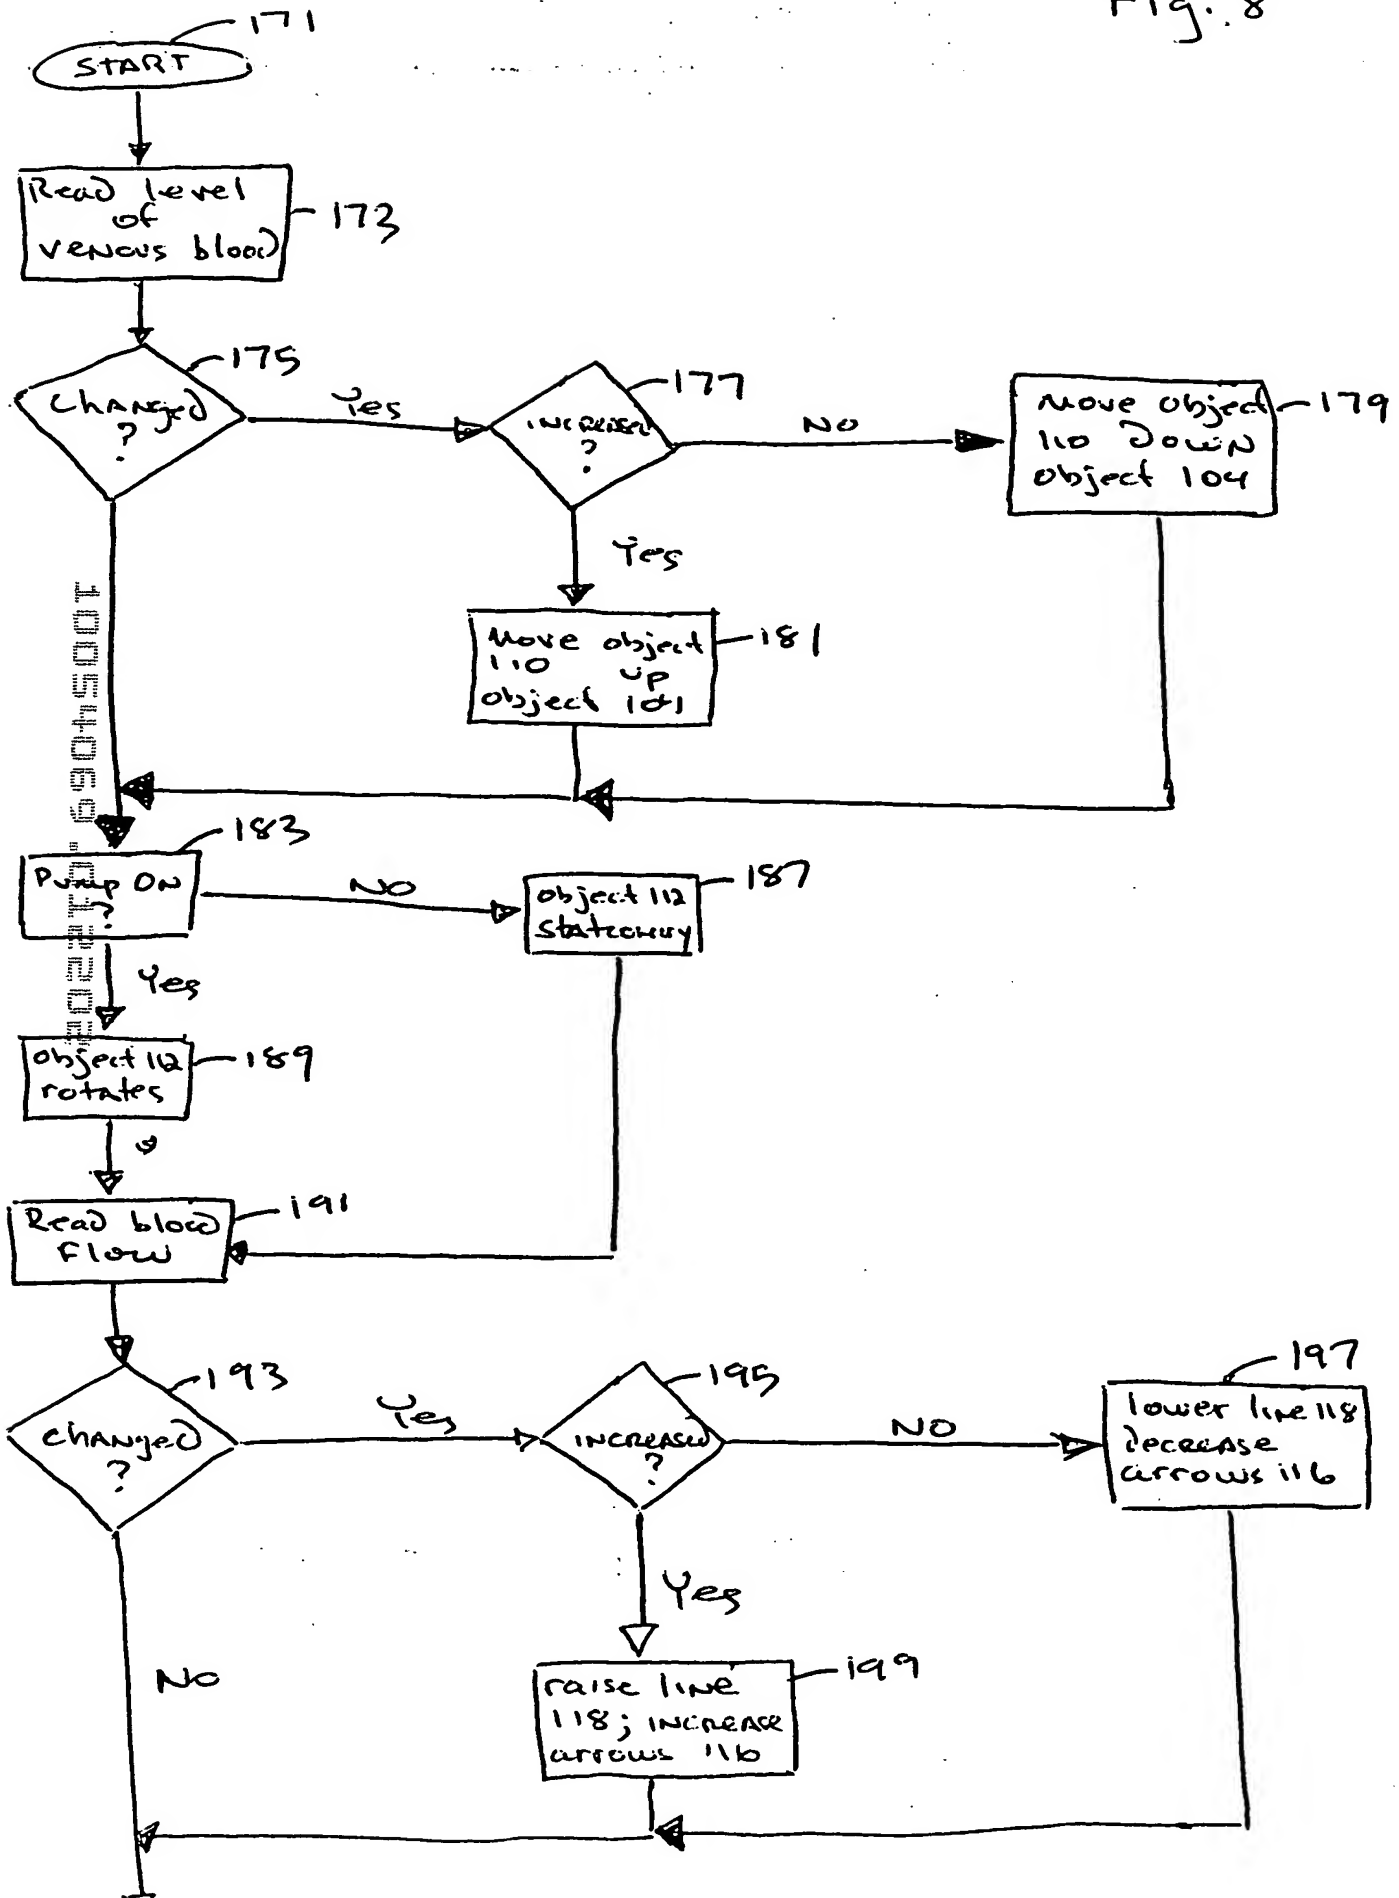
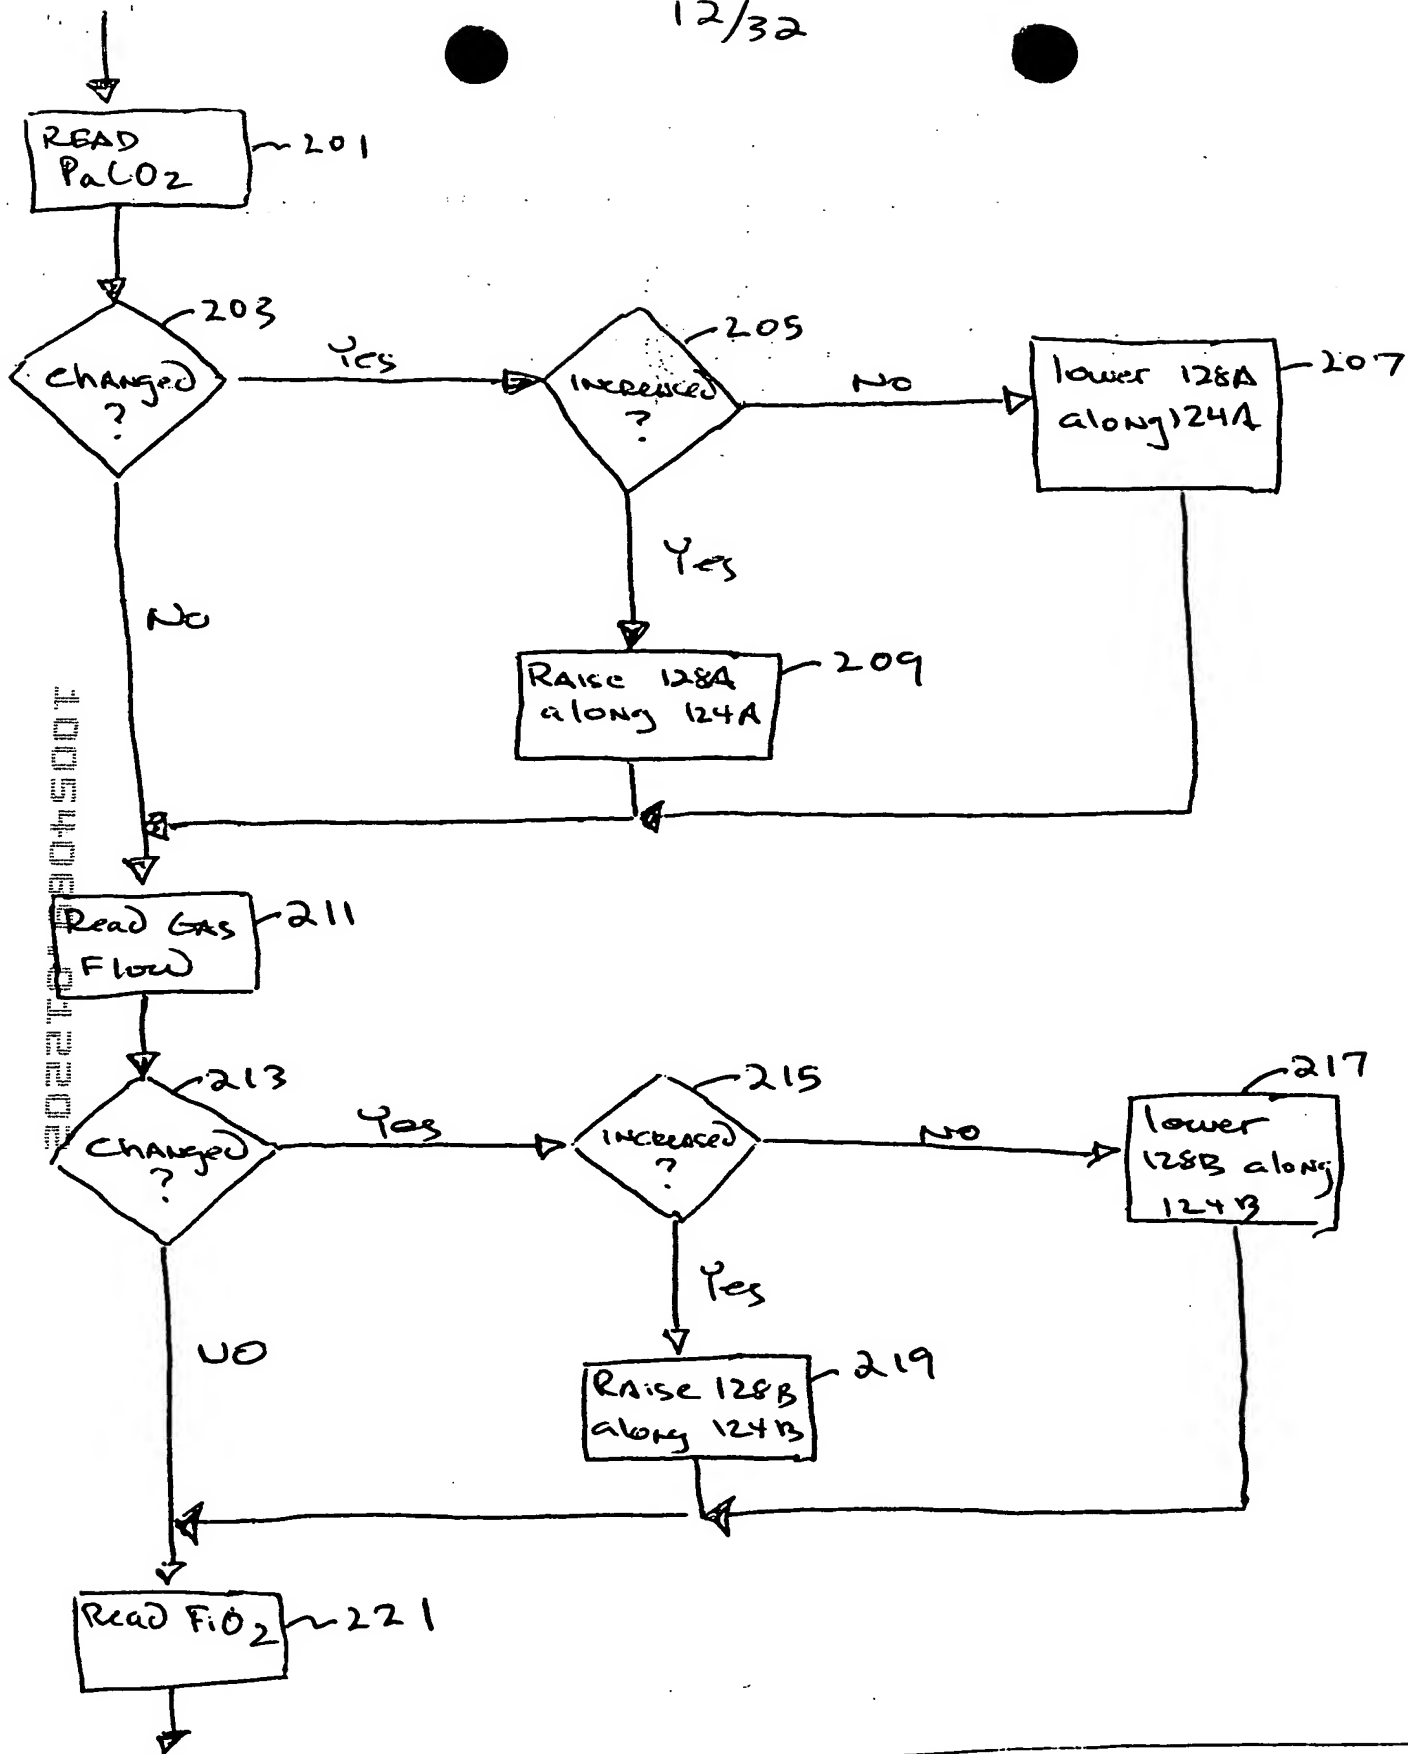


Fig. 8





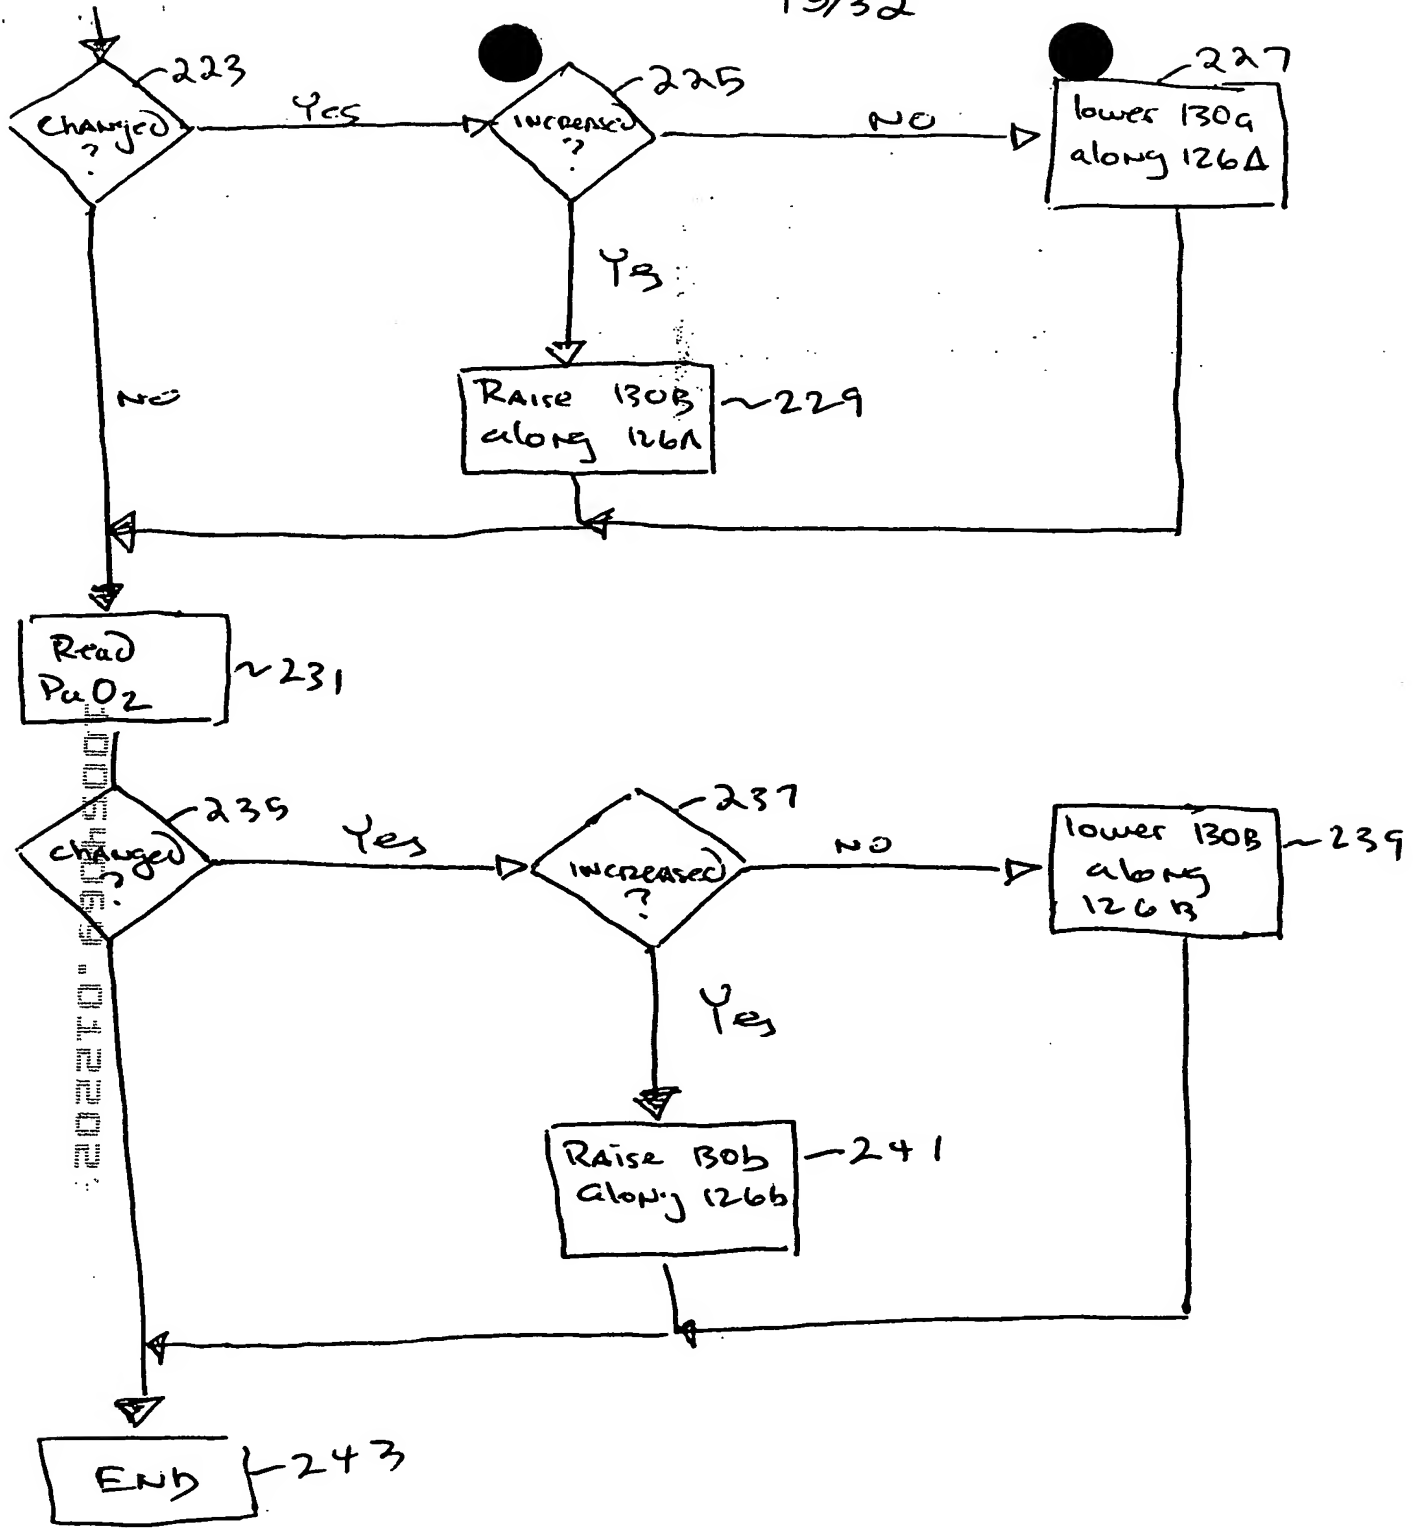


Fig. 9

Ventilator State Representation

140




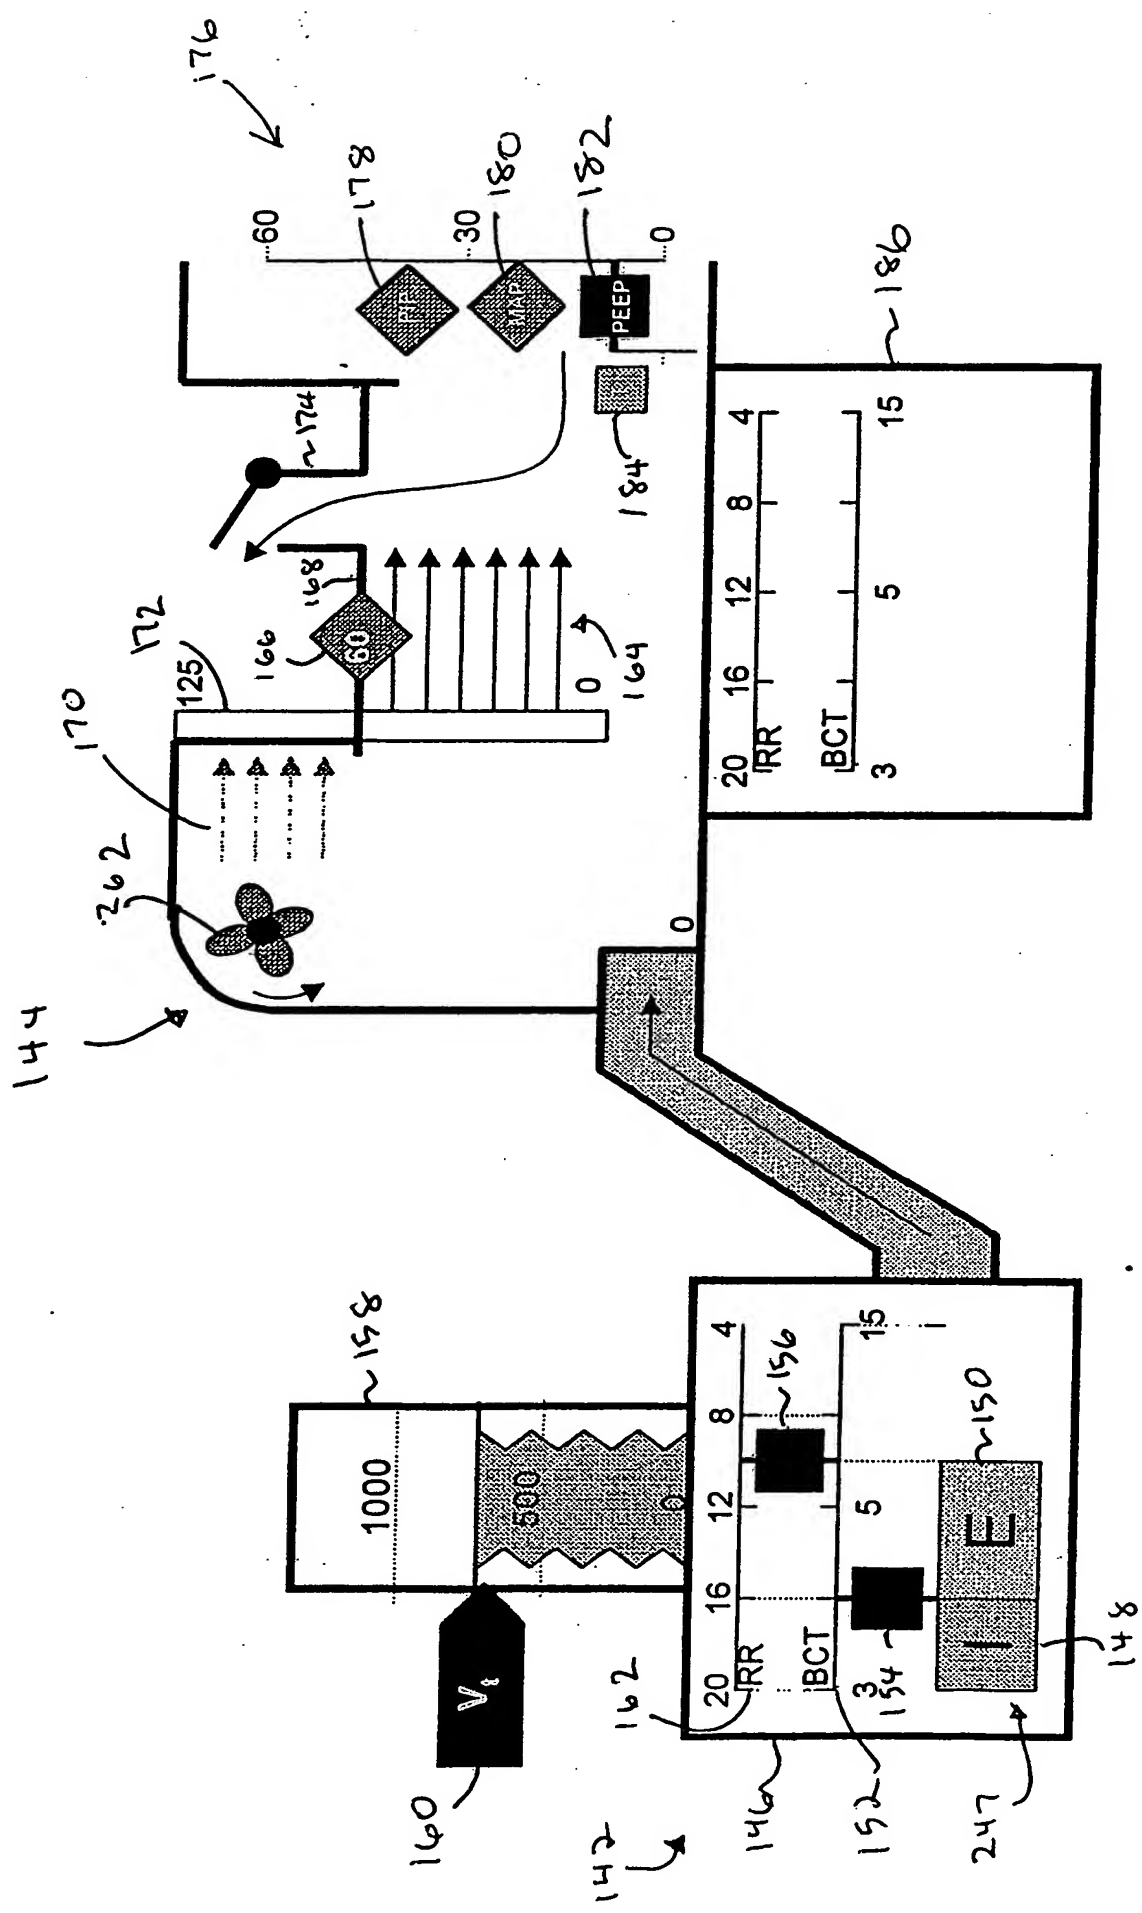


Fig. 10

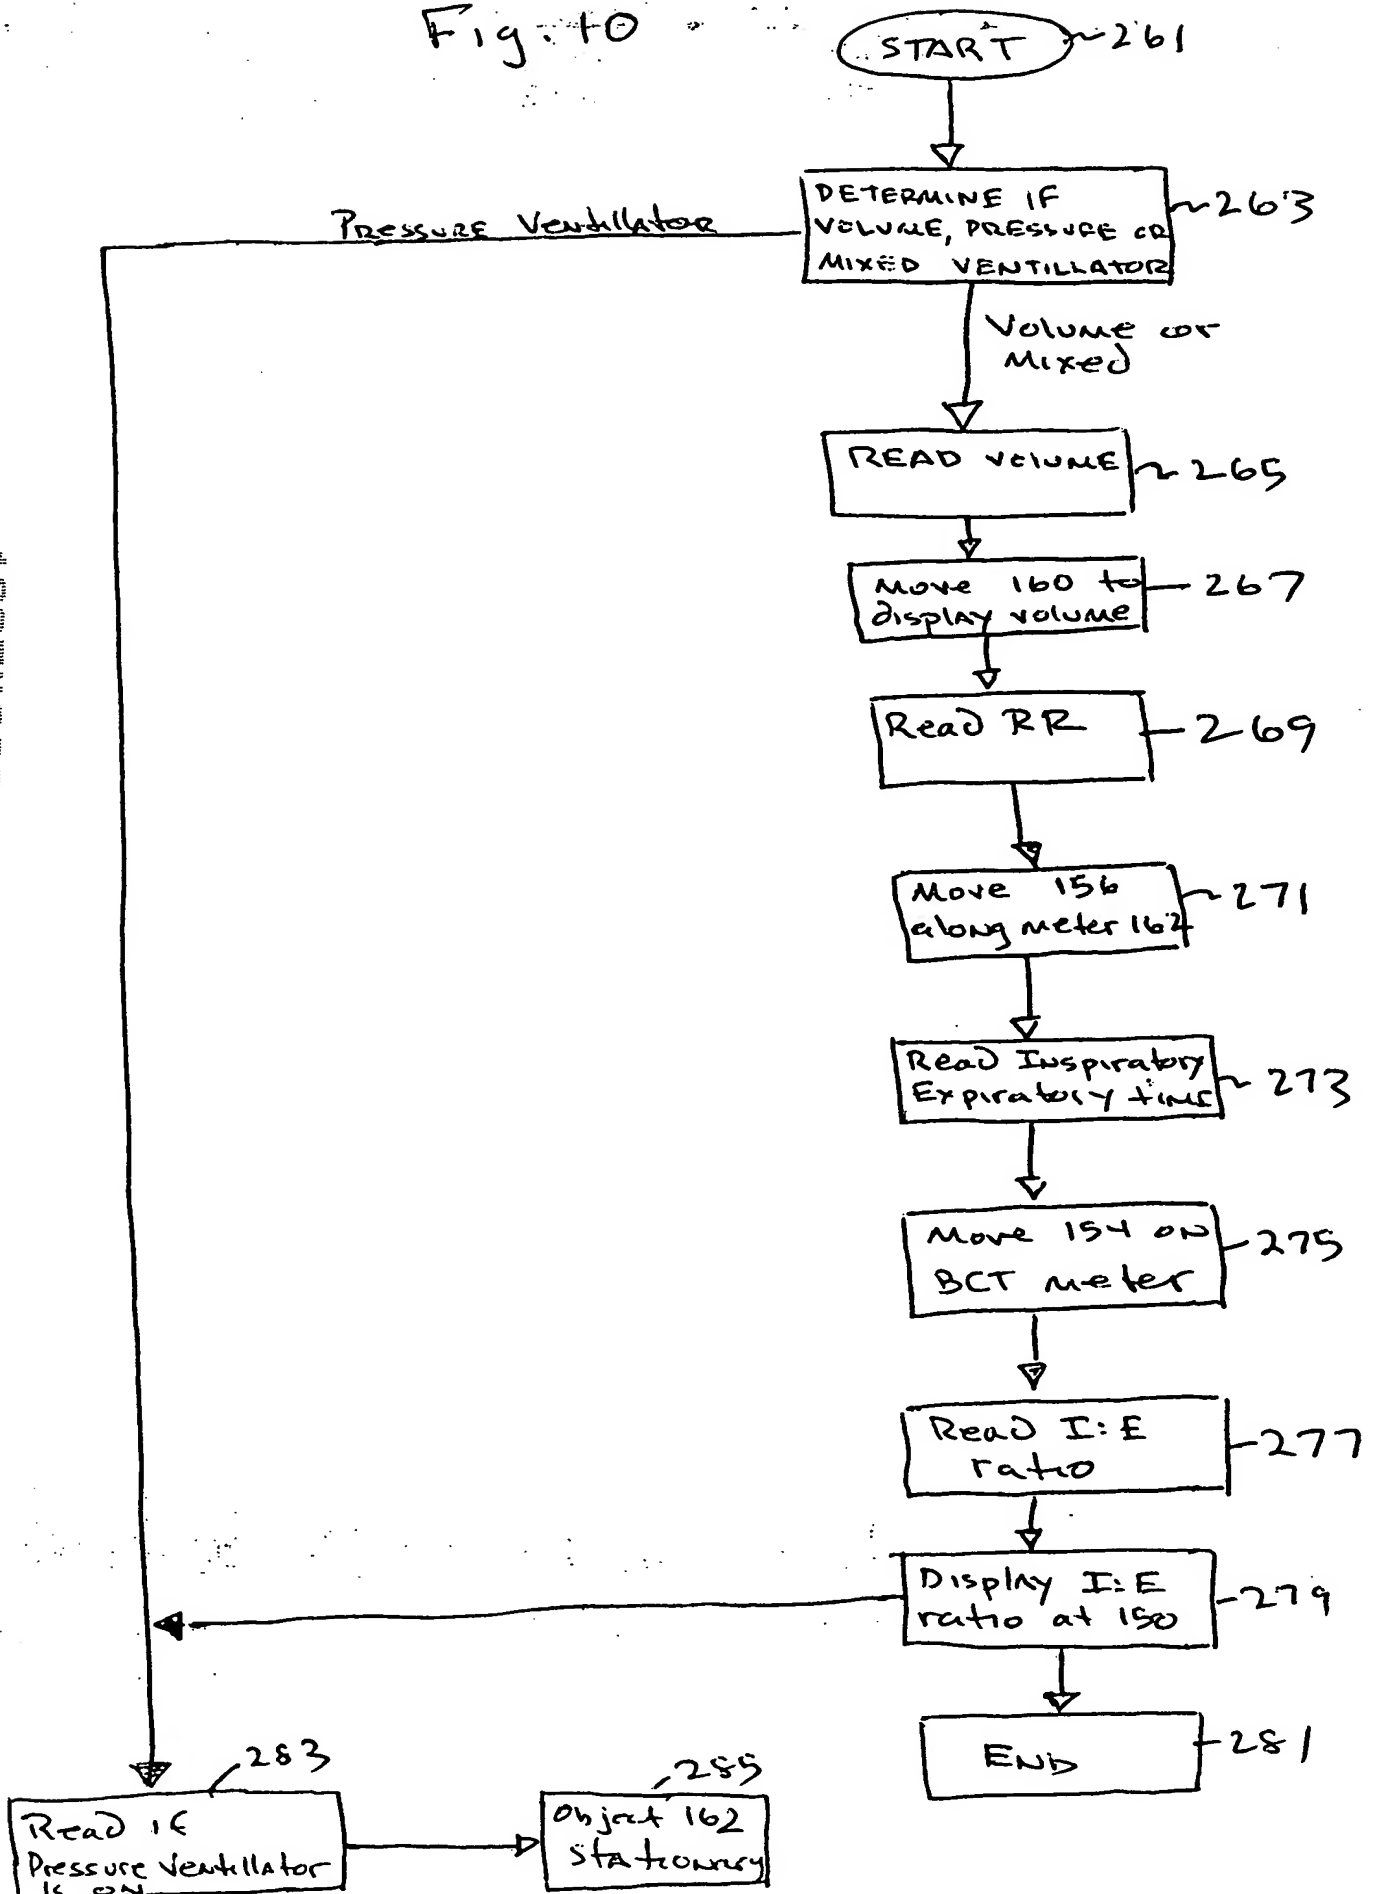


10054069-012202

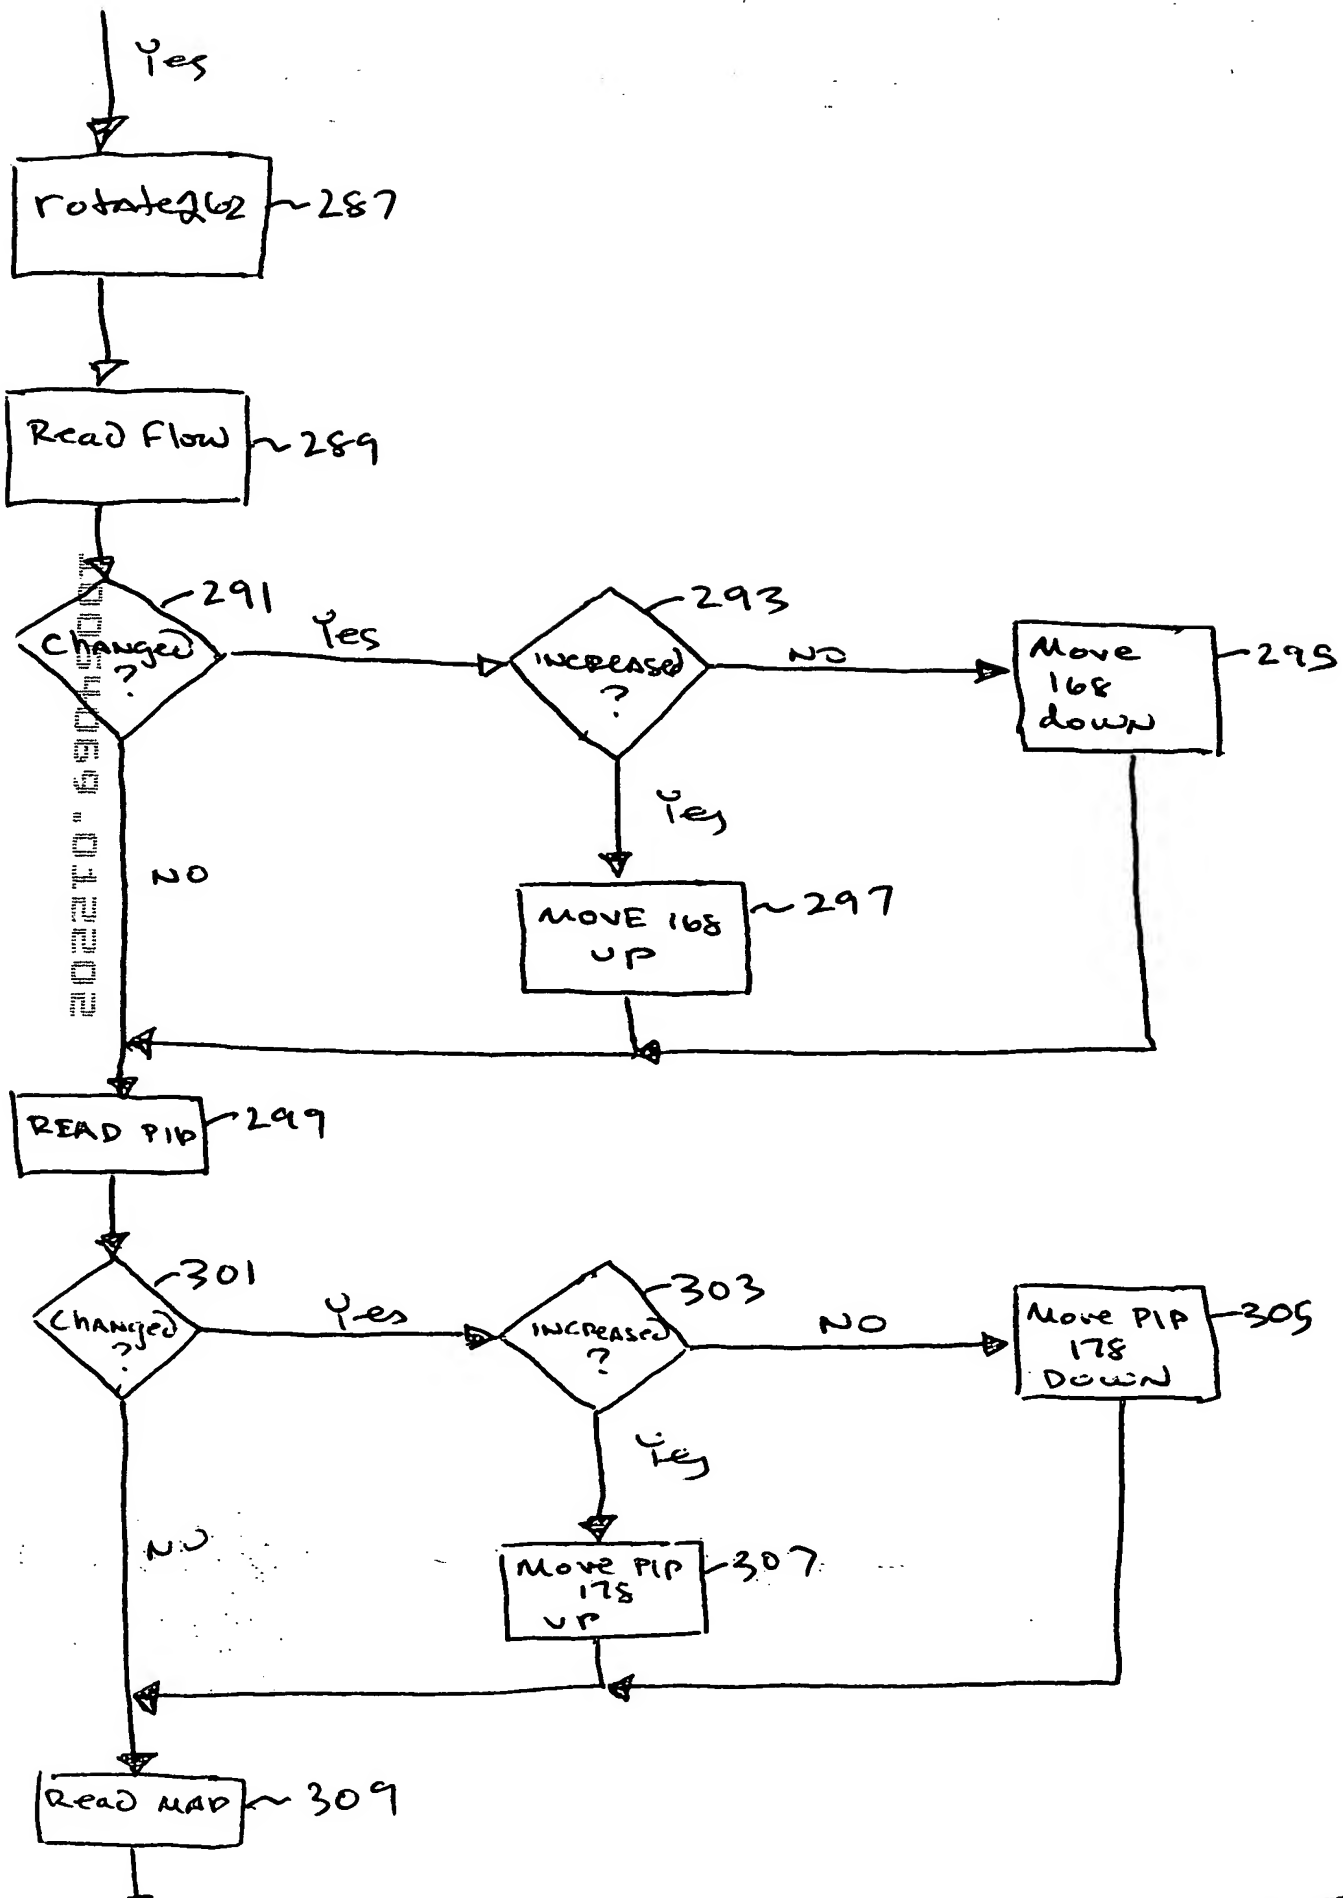

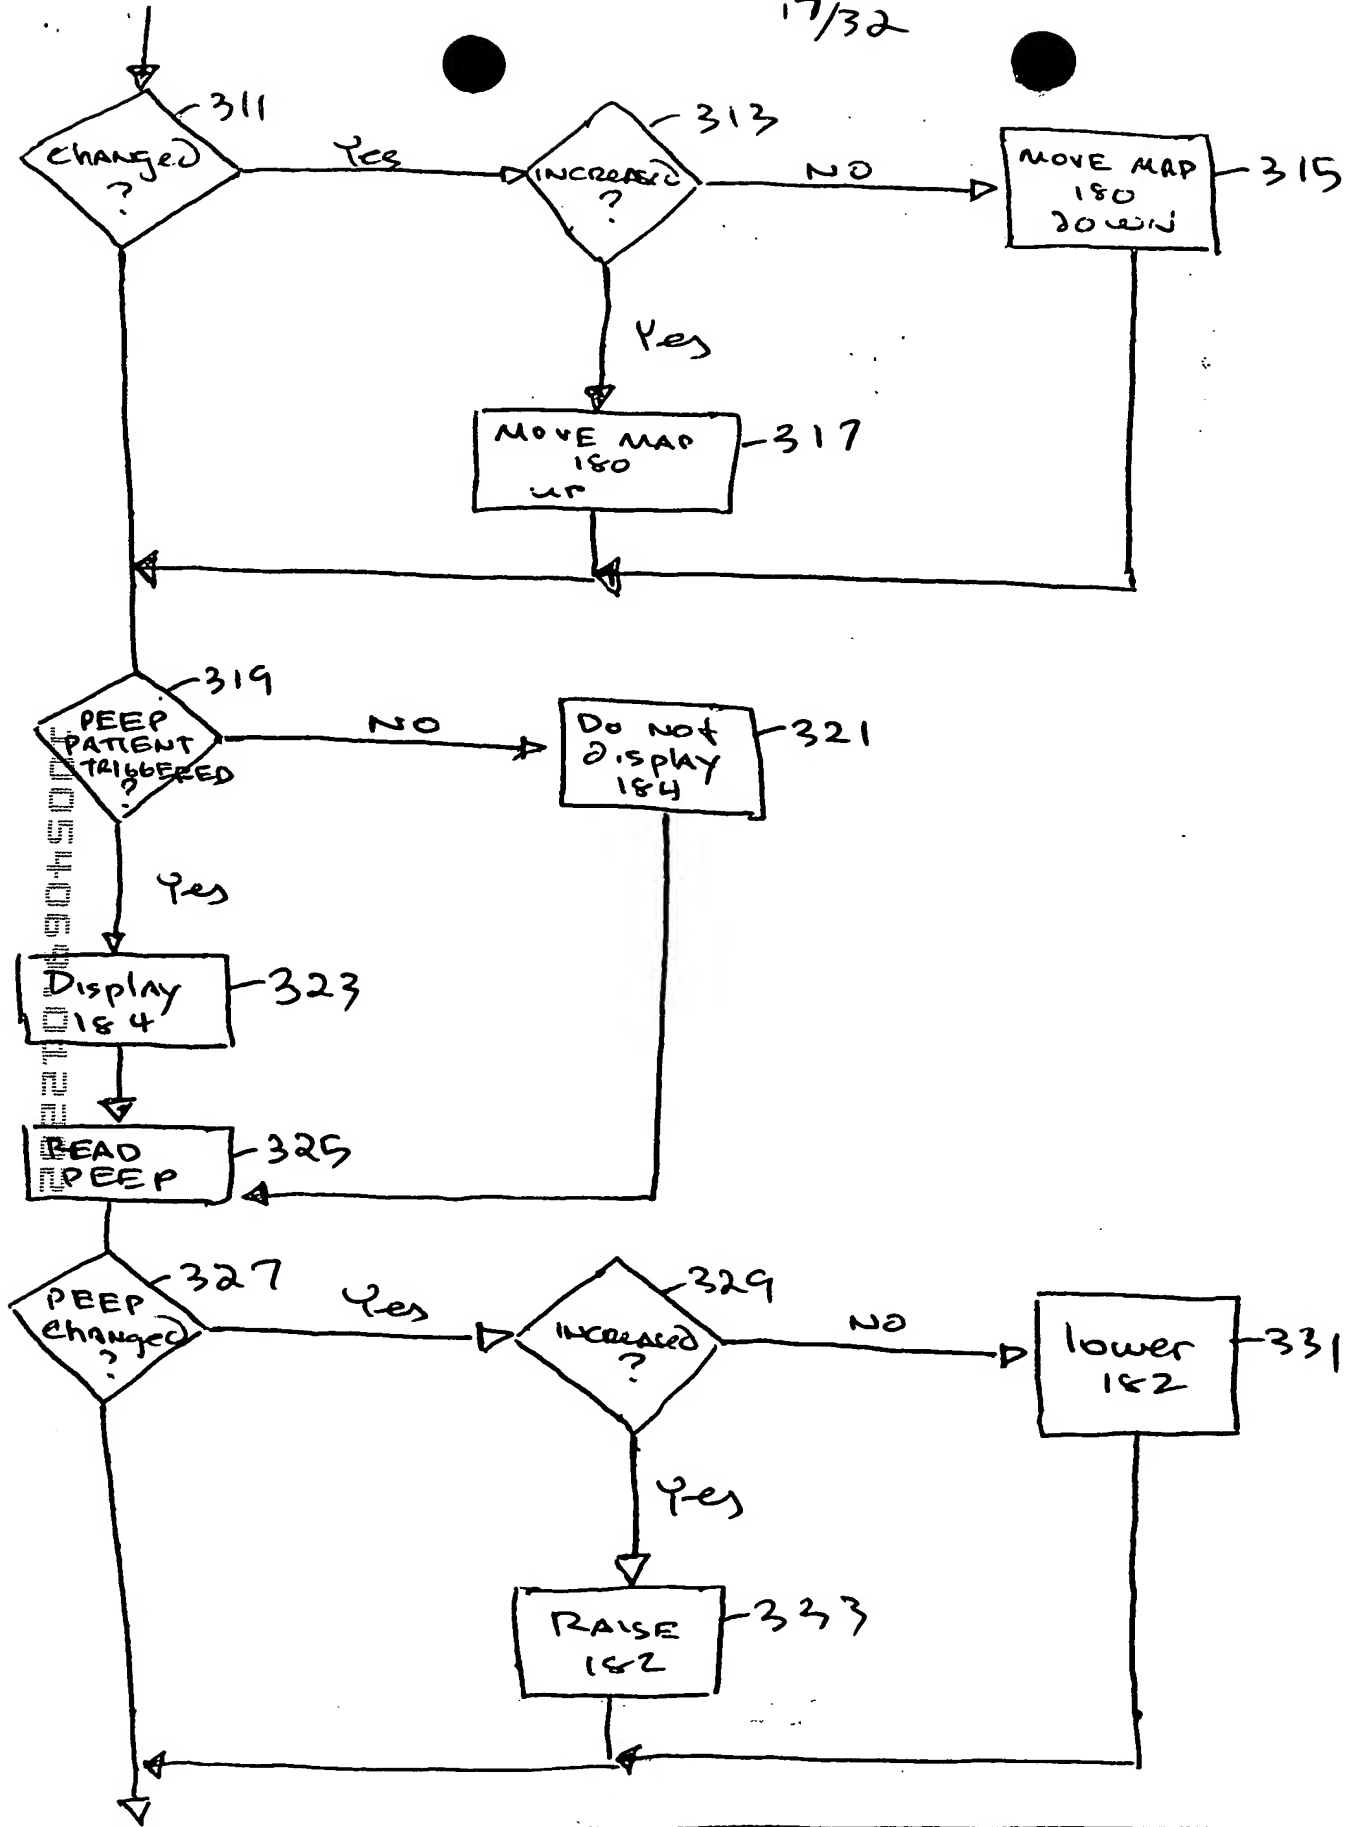

18/32

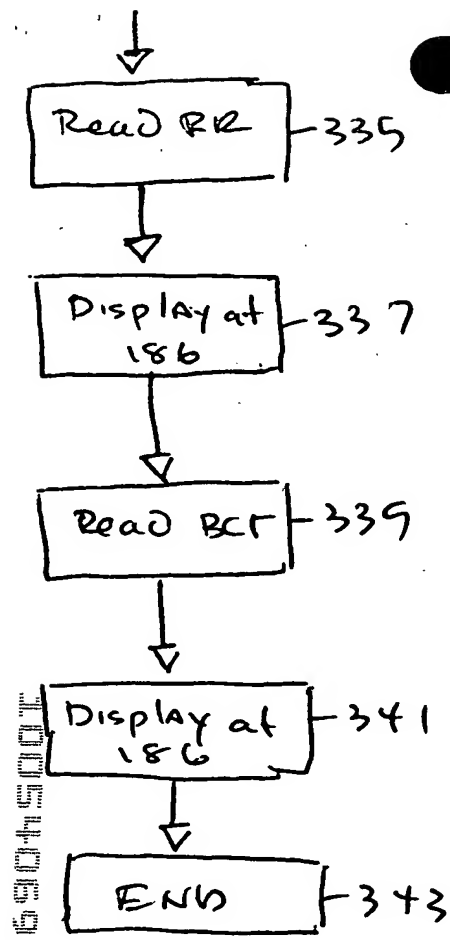

2022-10-10 10:54:06

10054069-012202

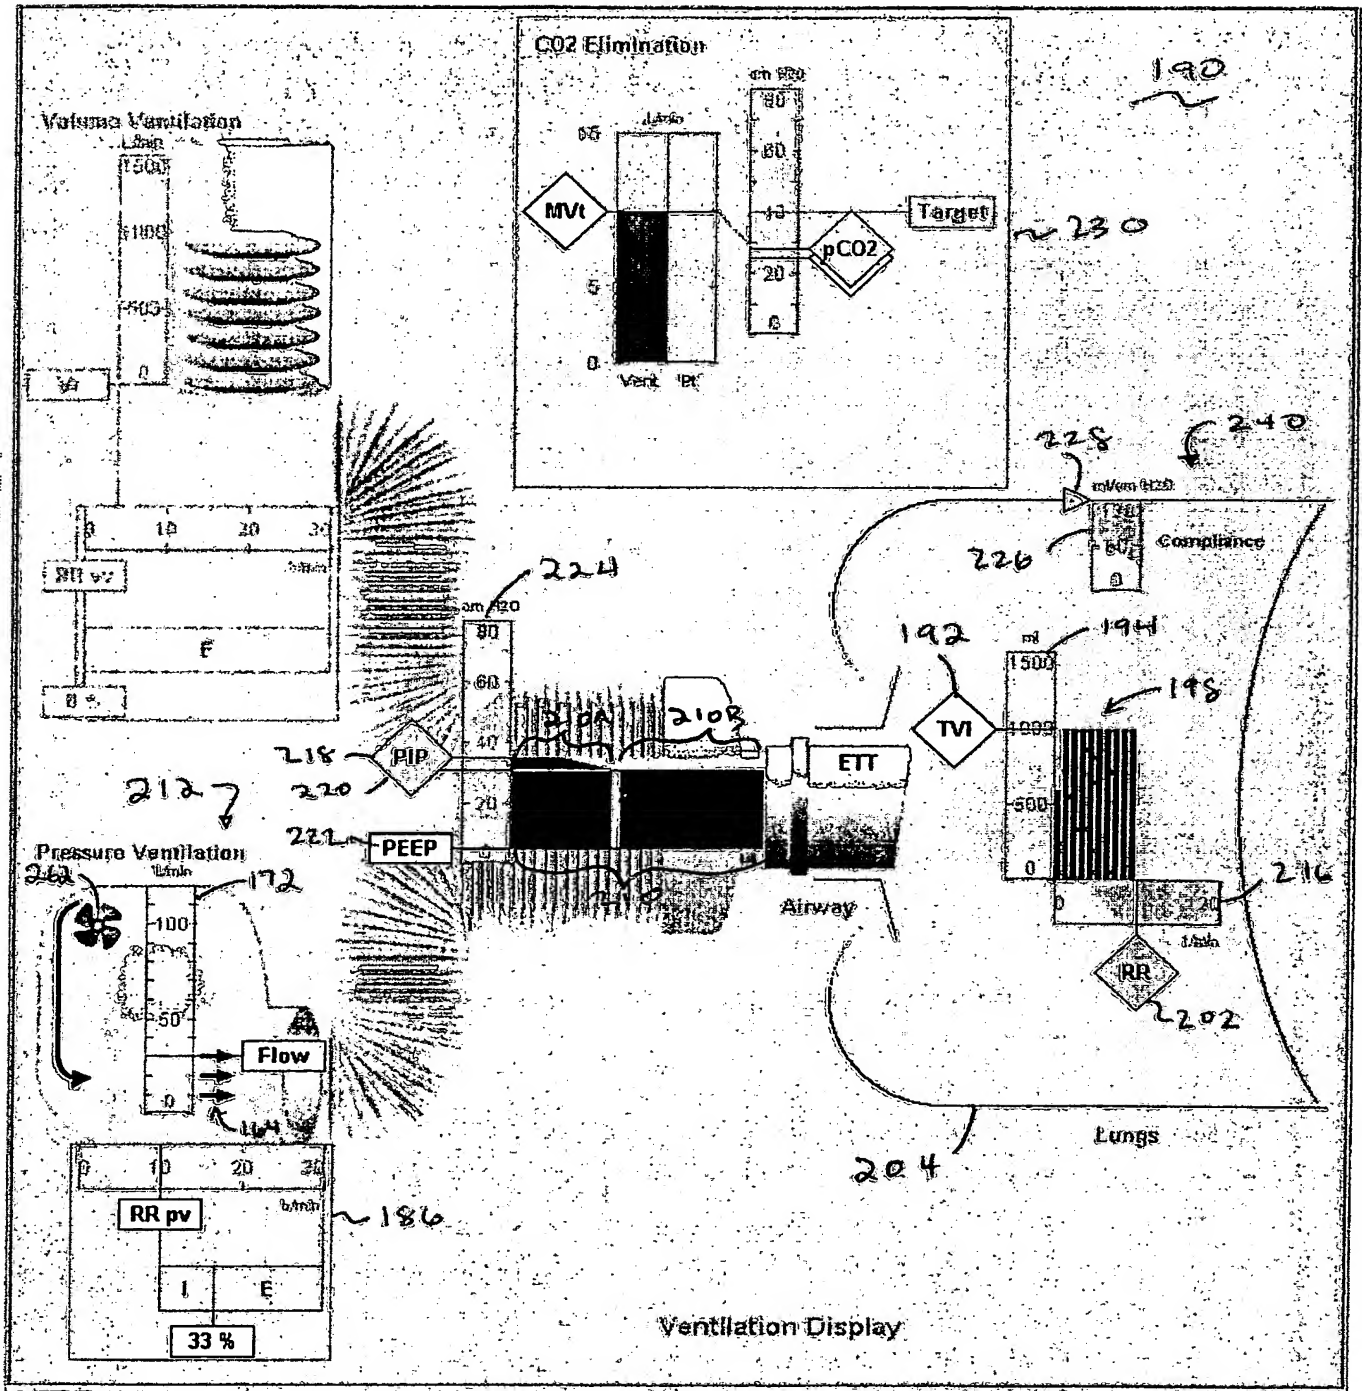


Fig. 11

10054069-012202

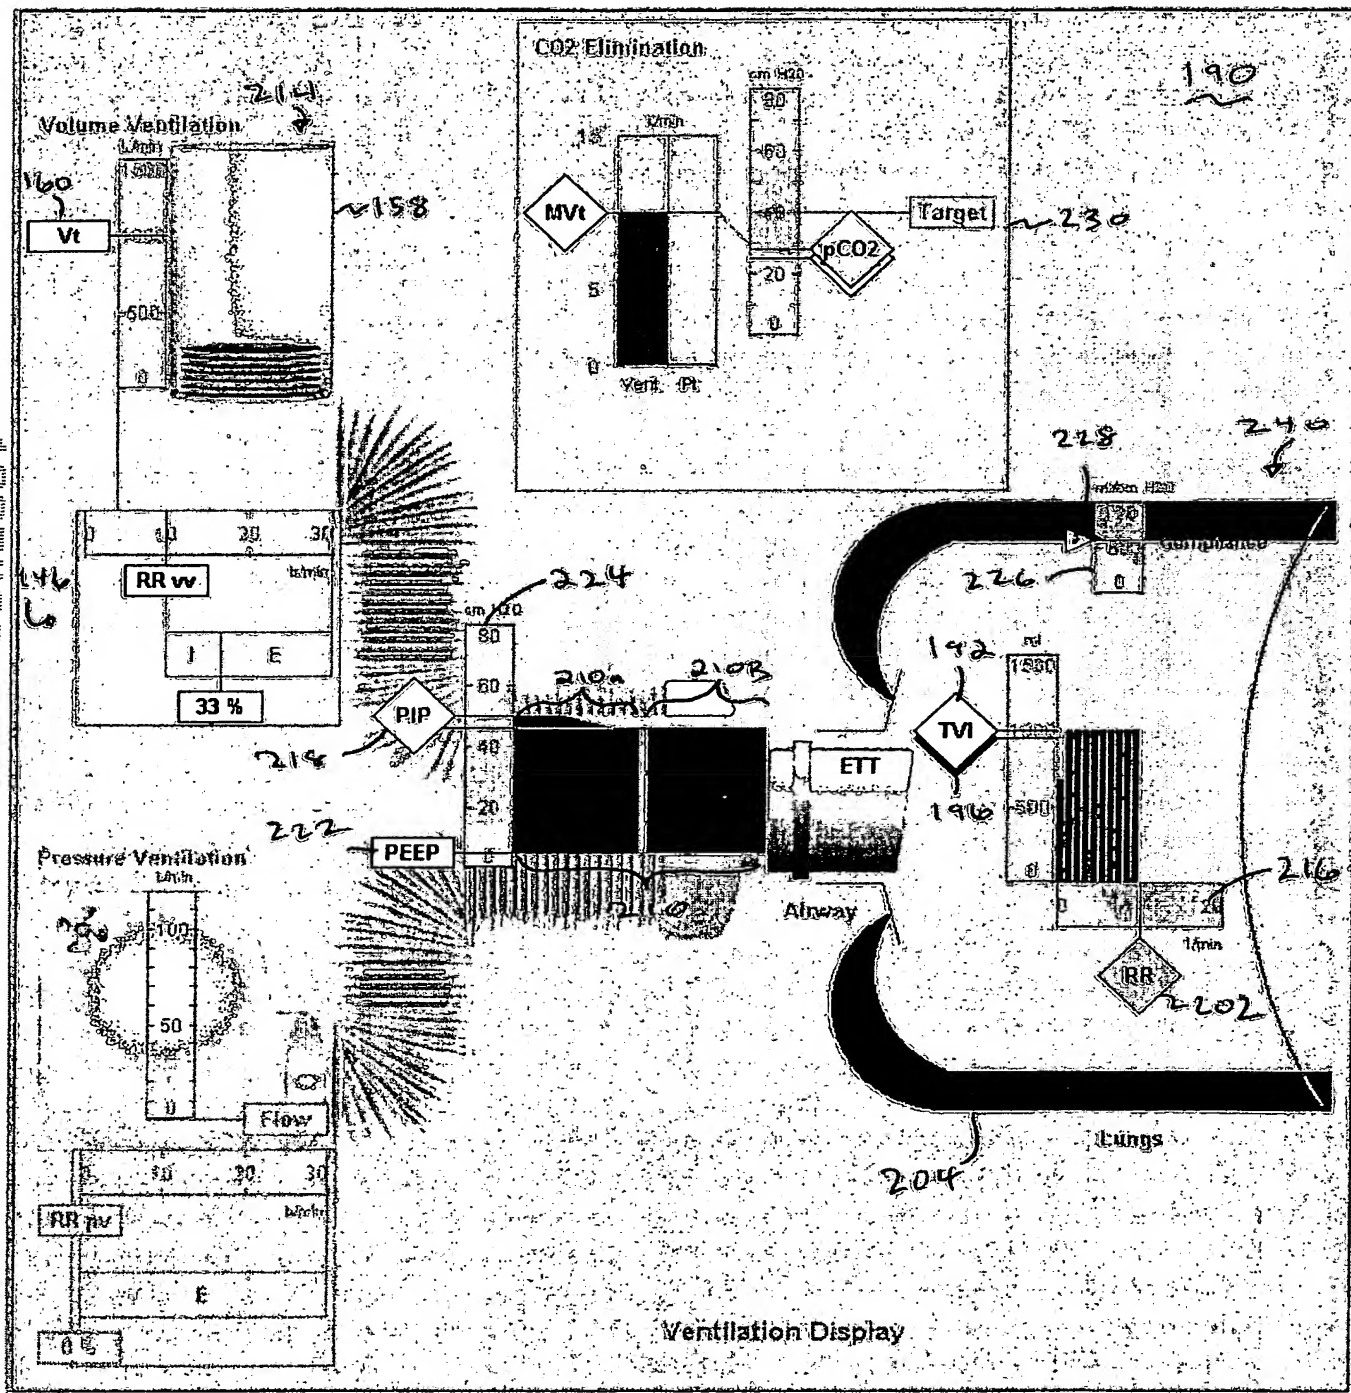


Fig. 12

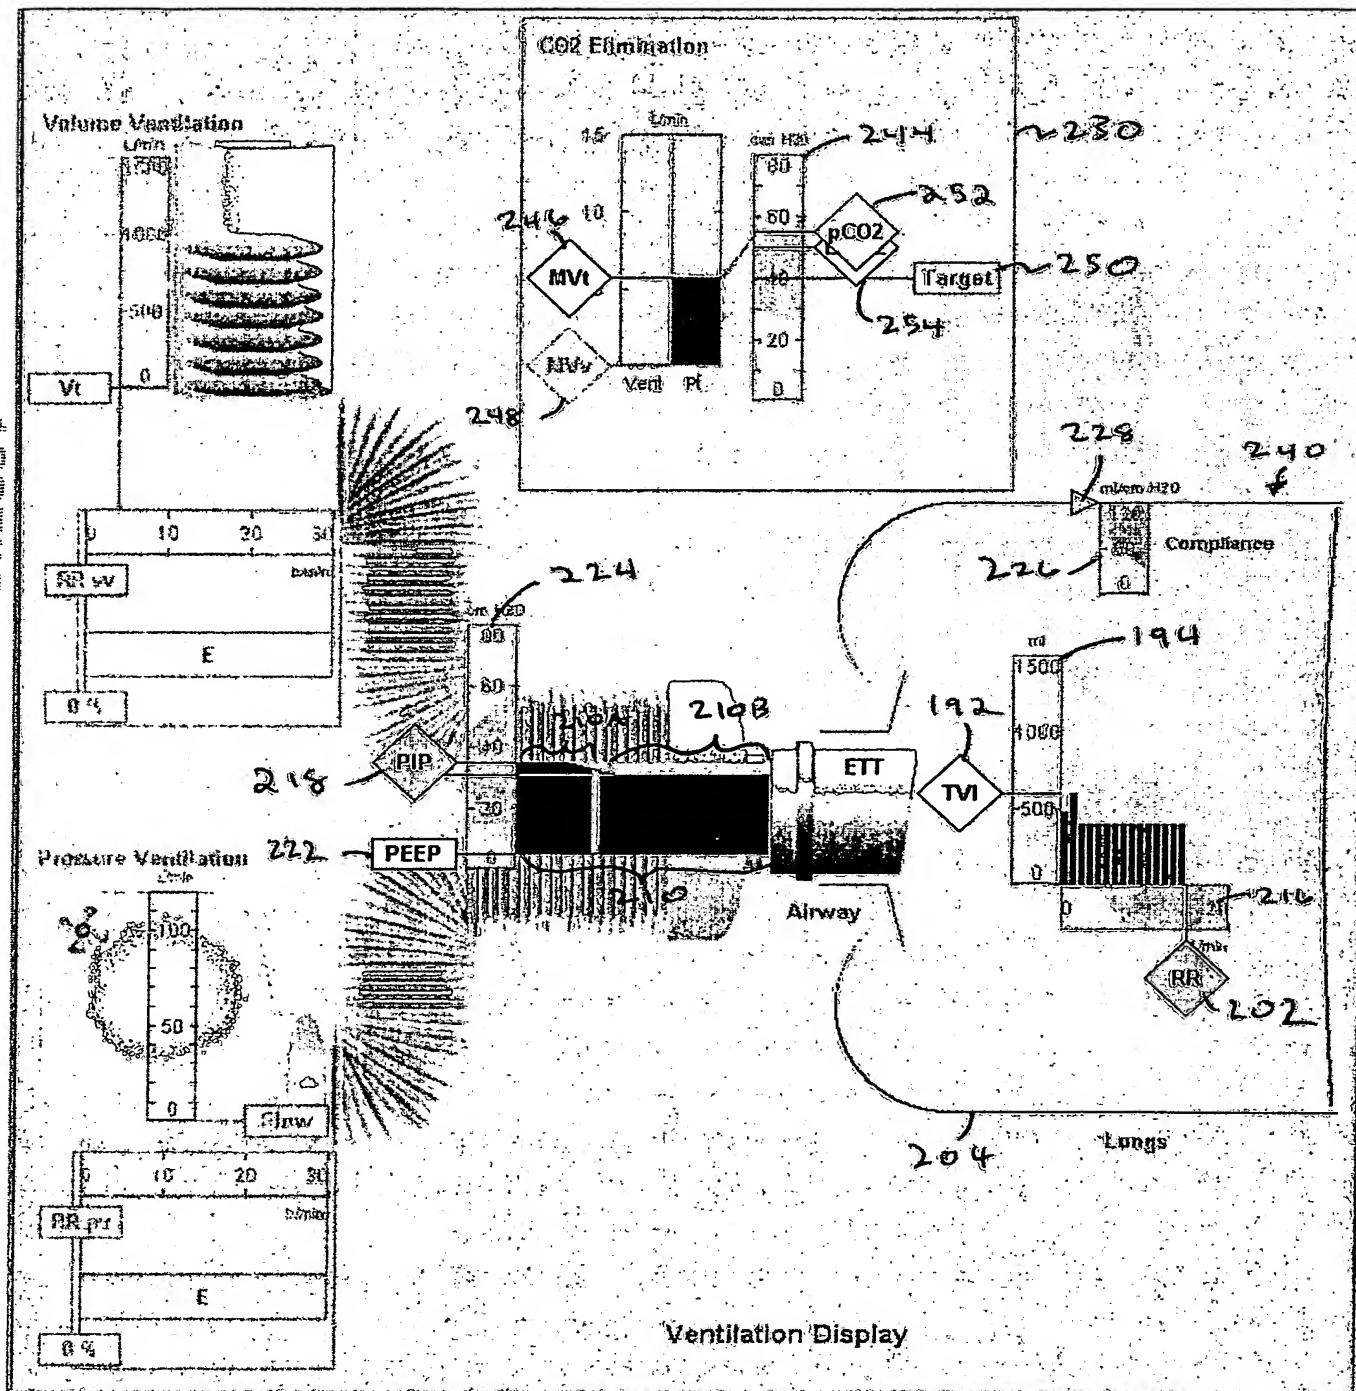
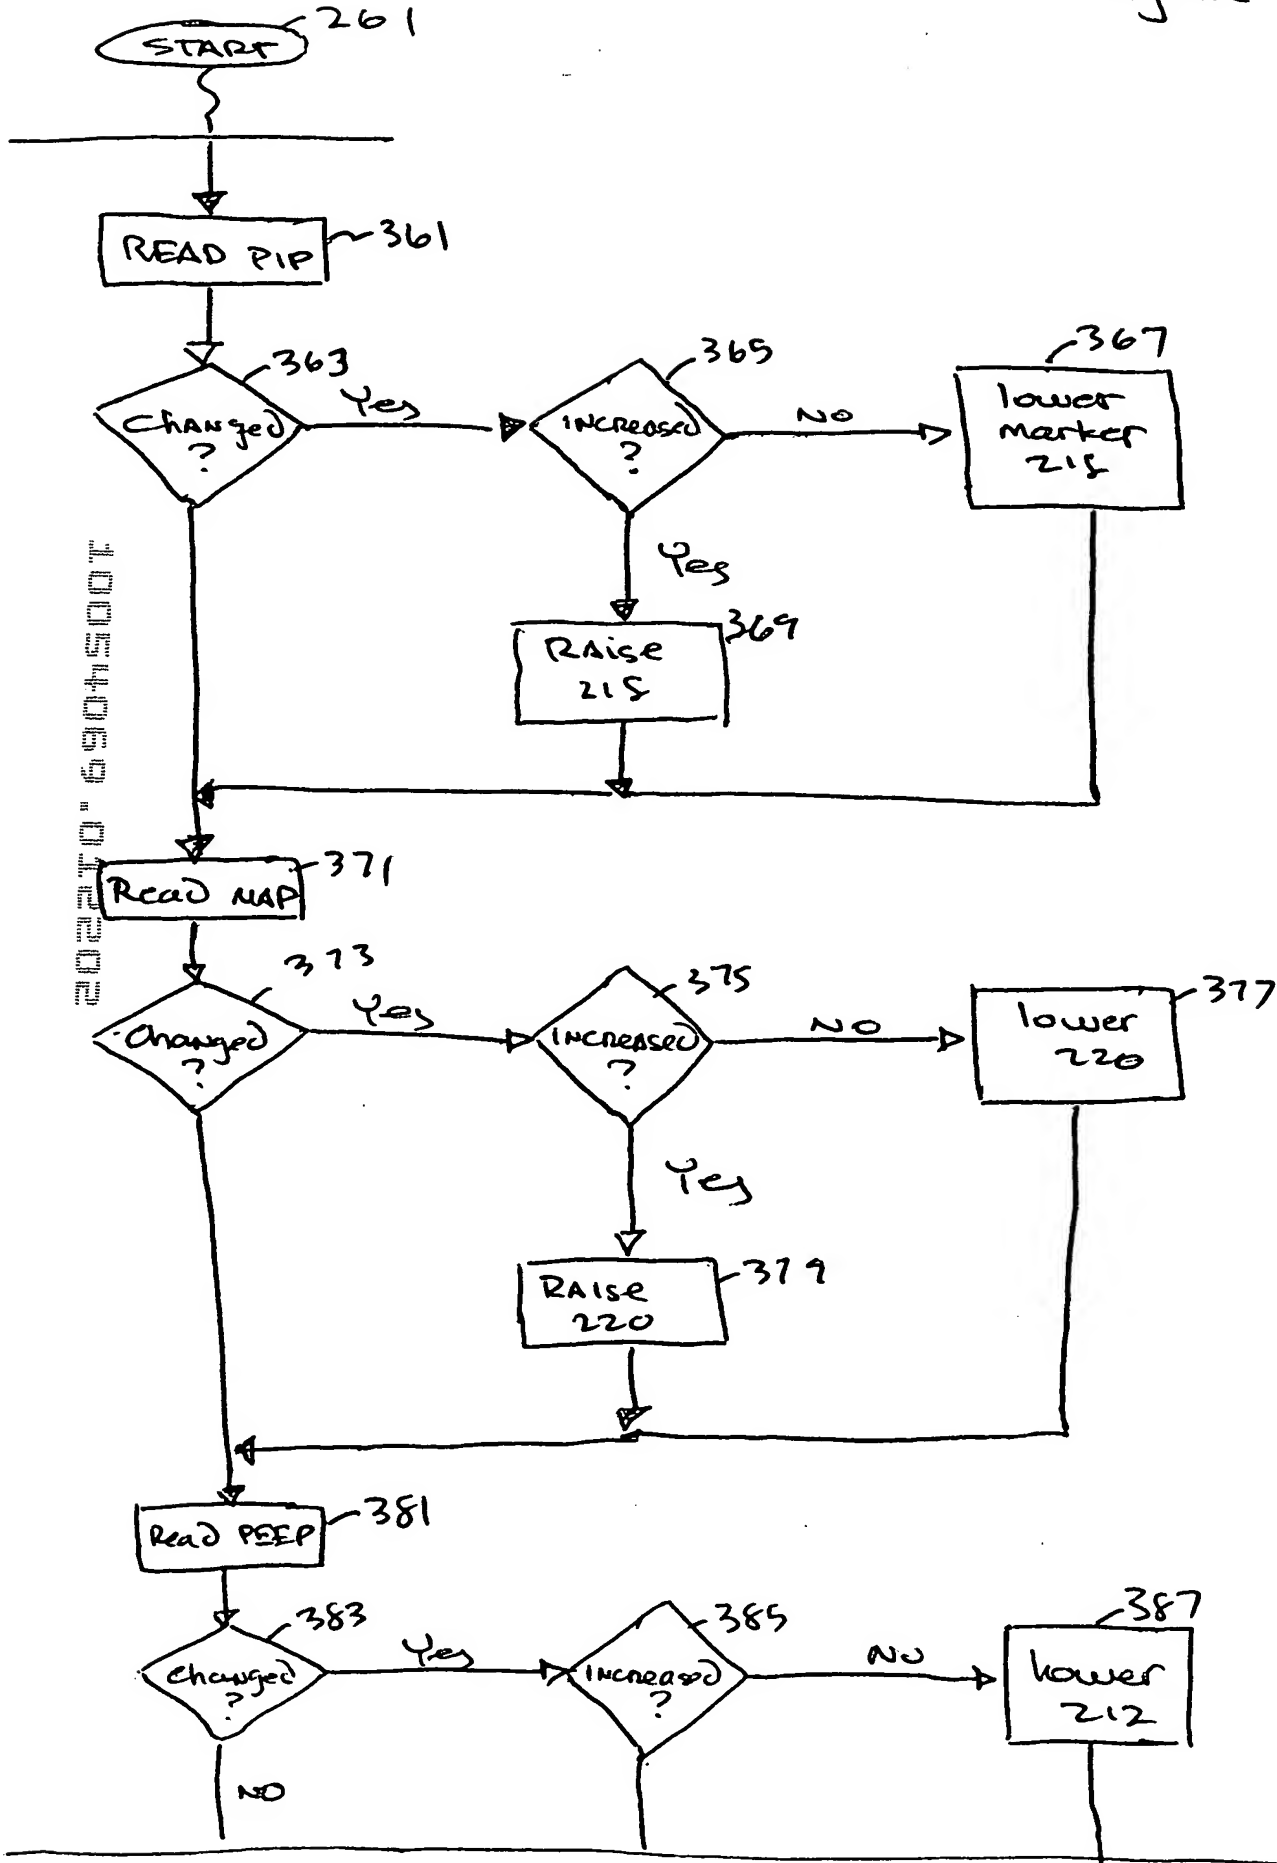
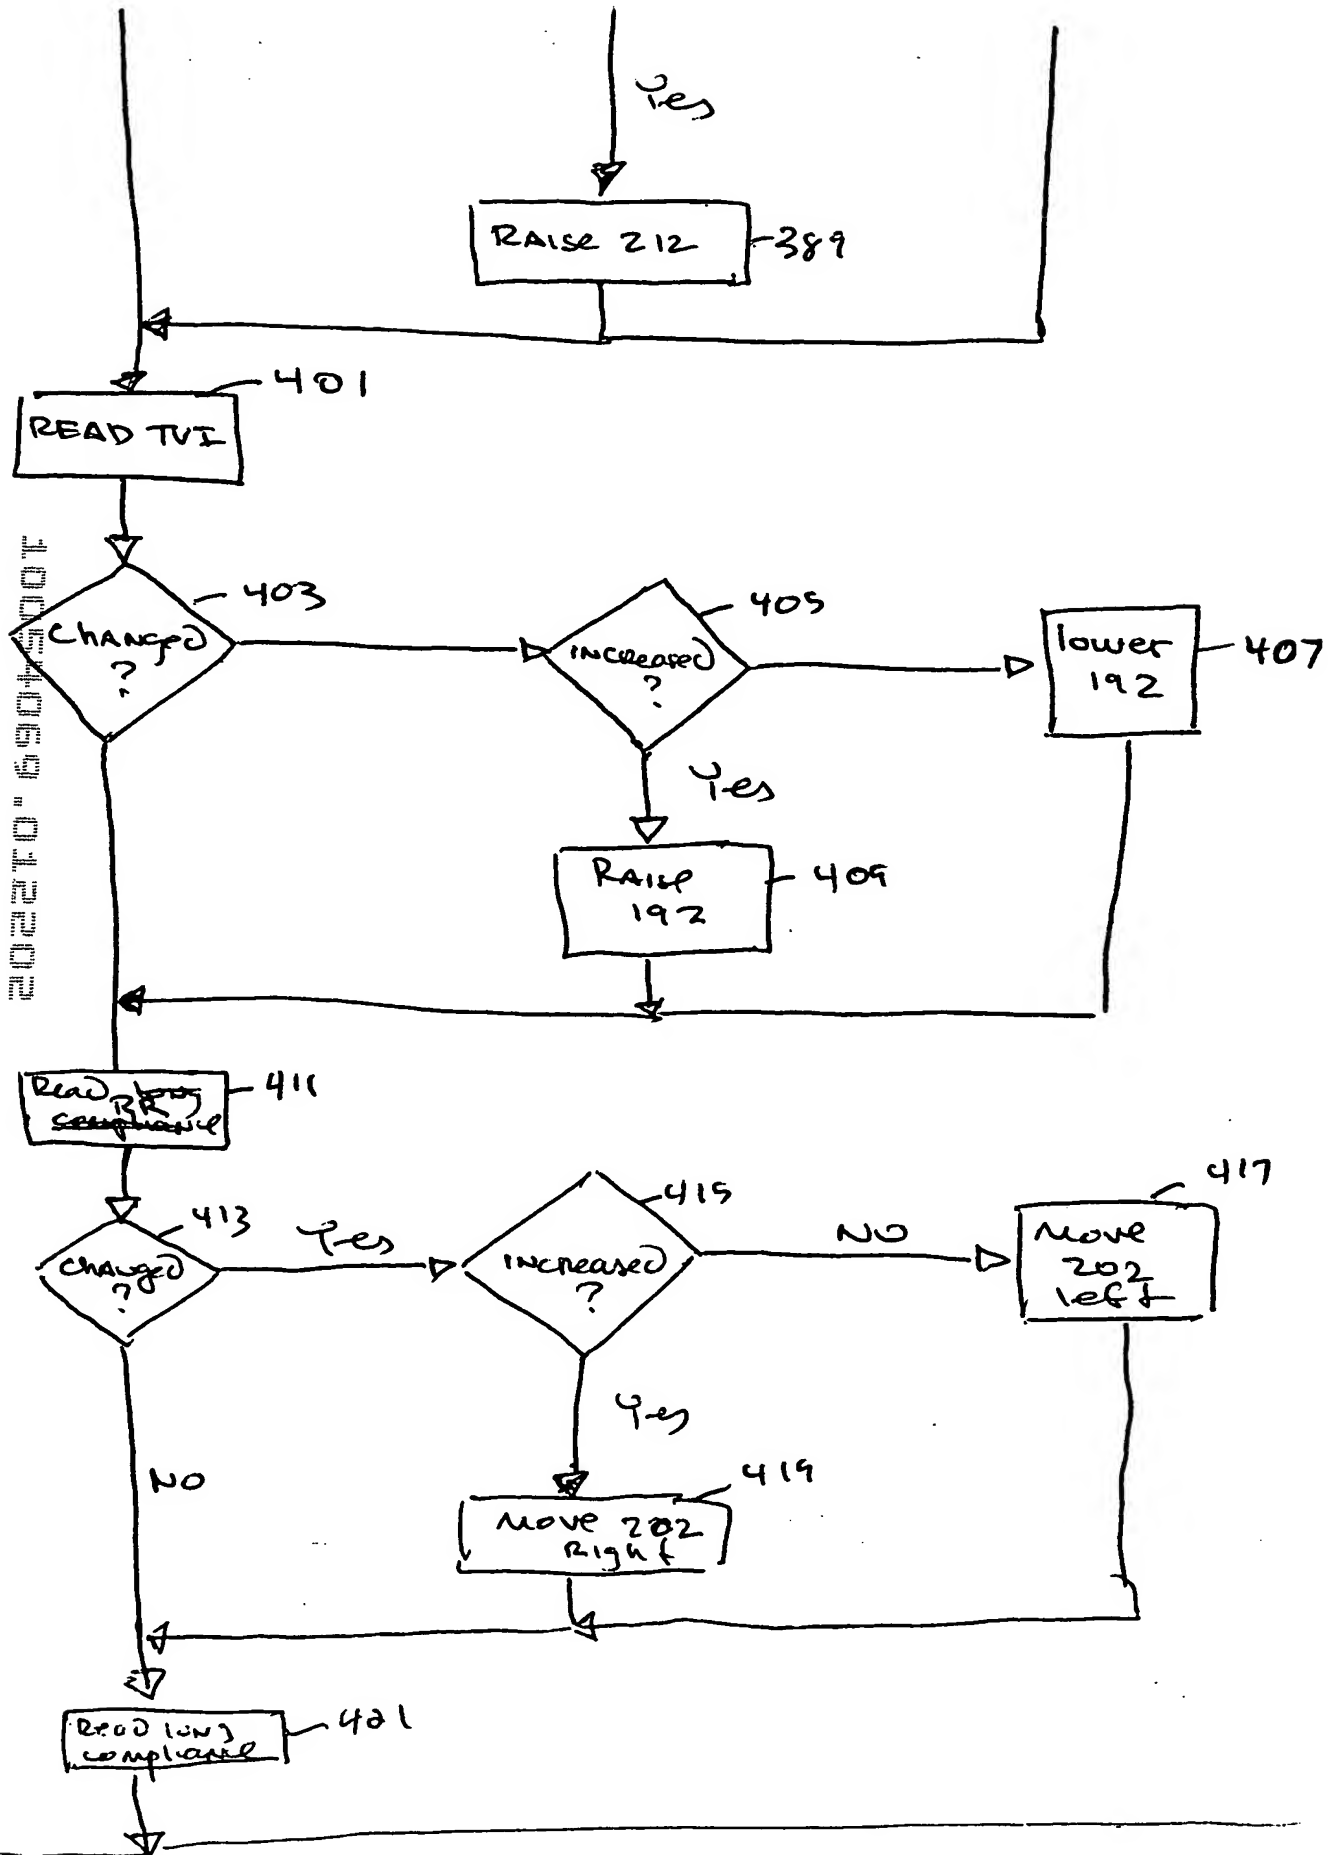
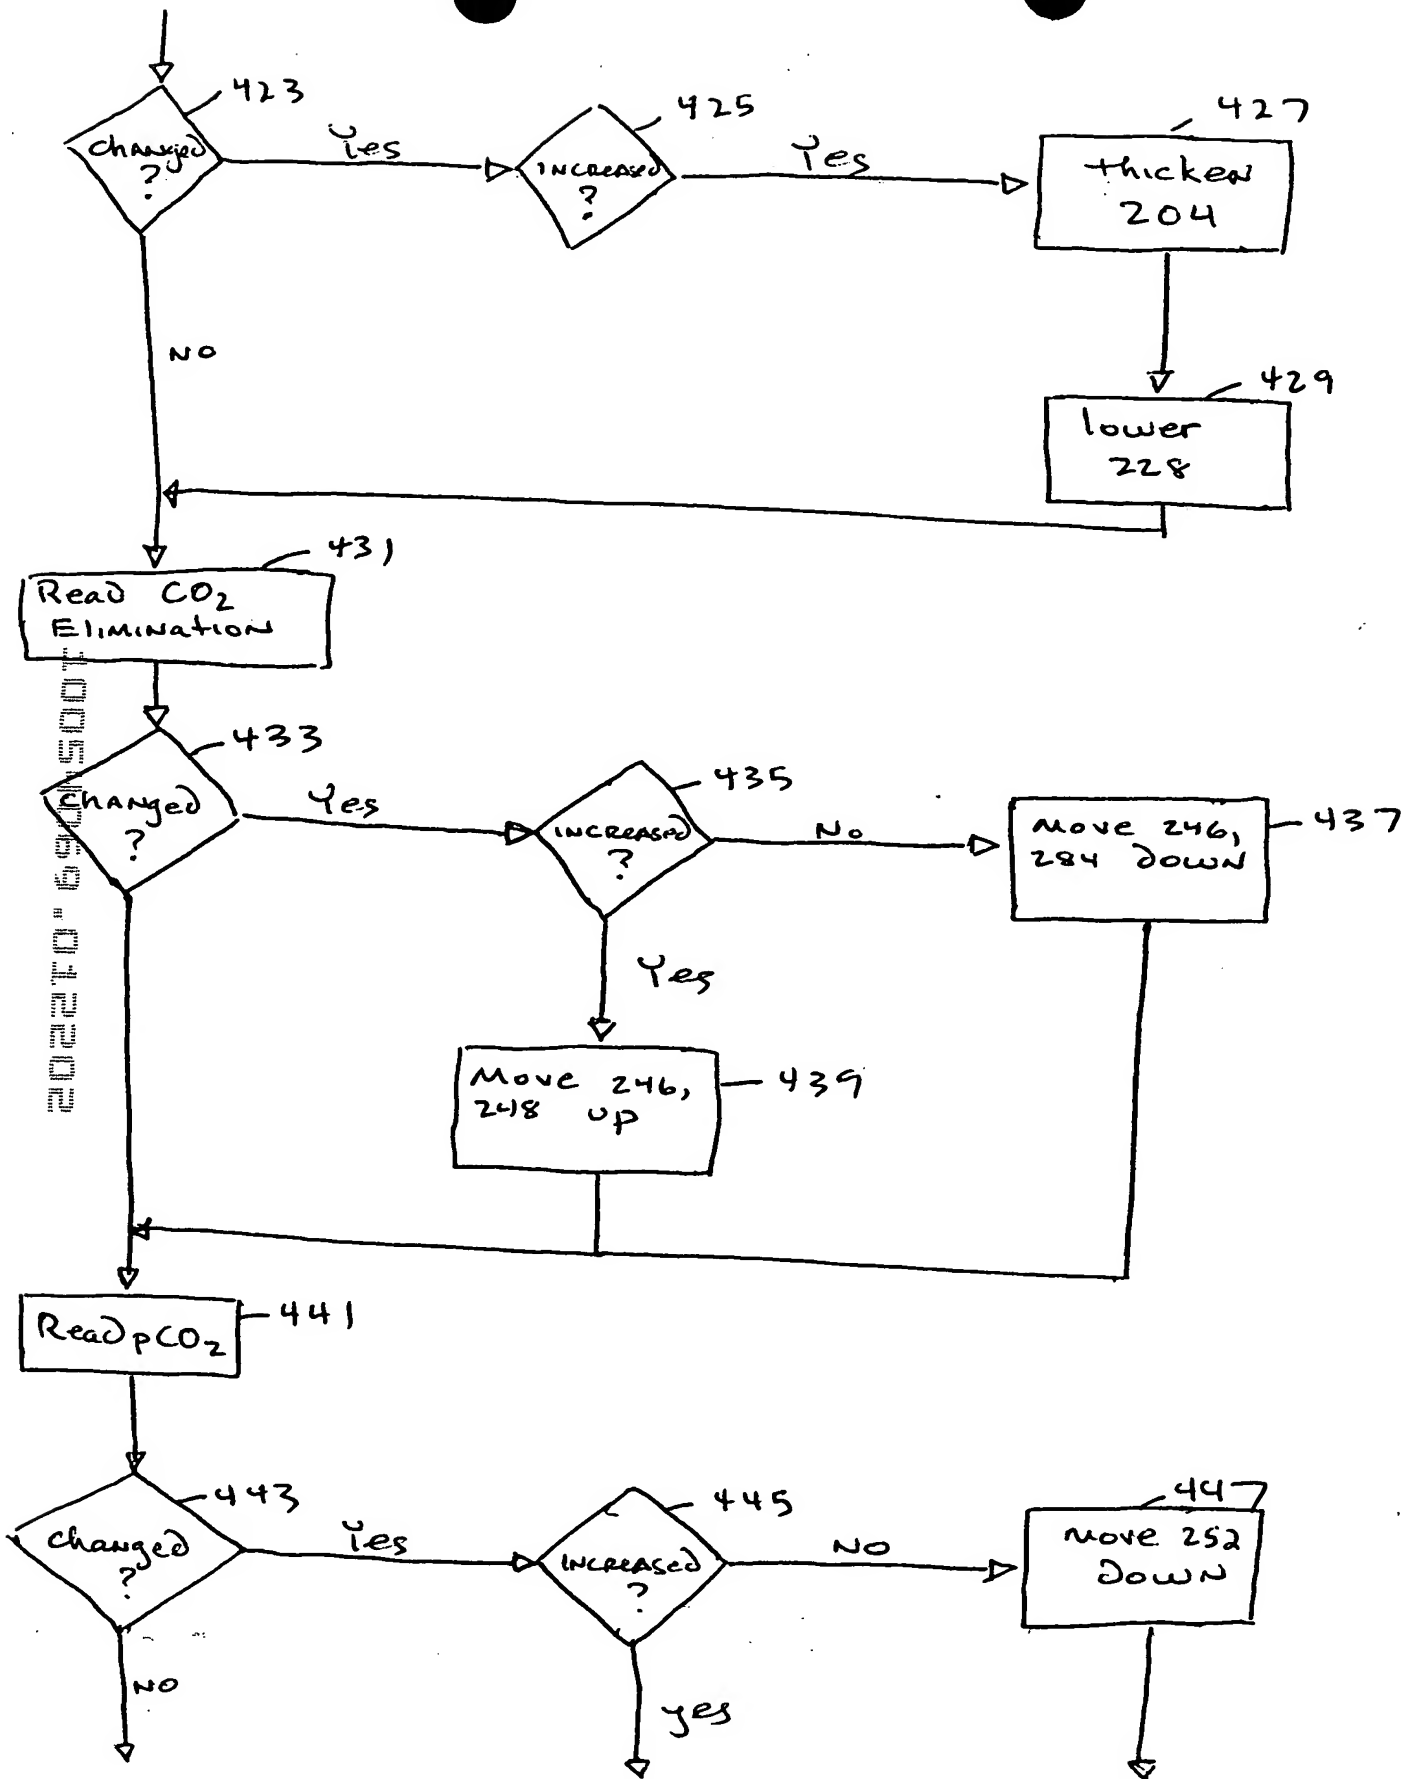


Figure 14







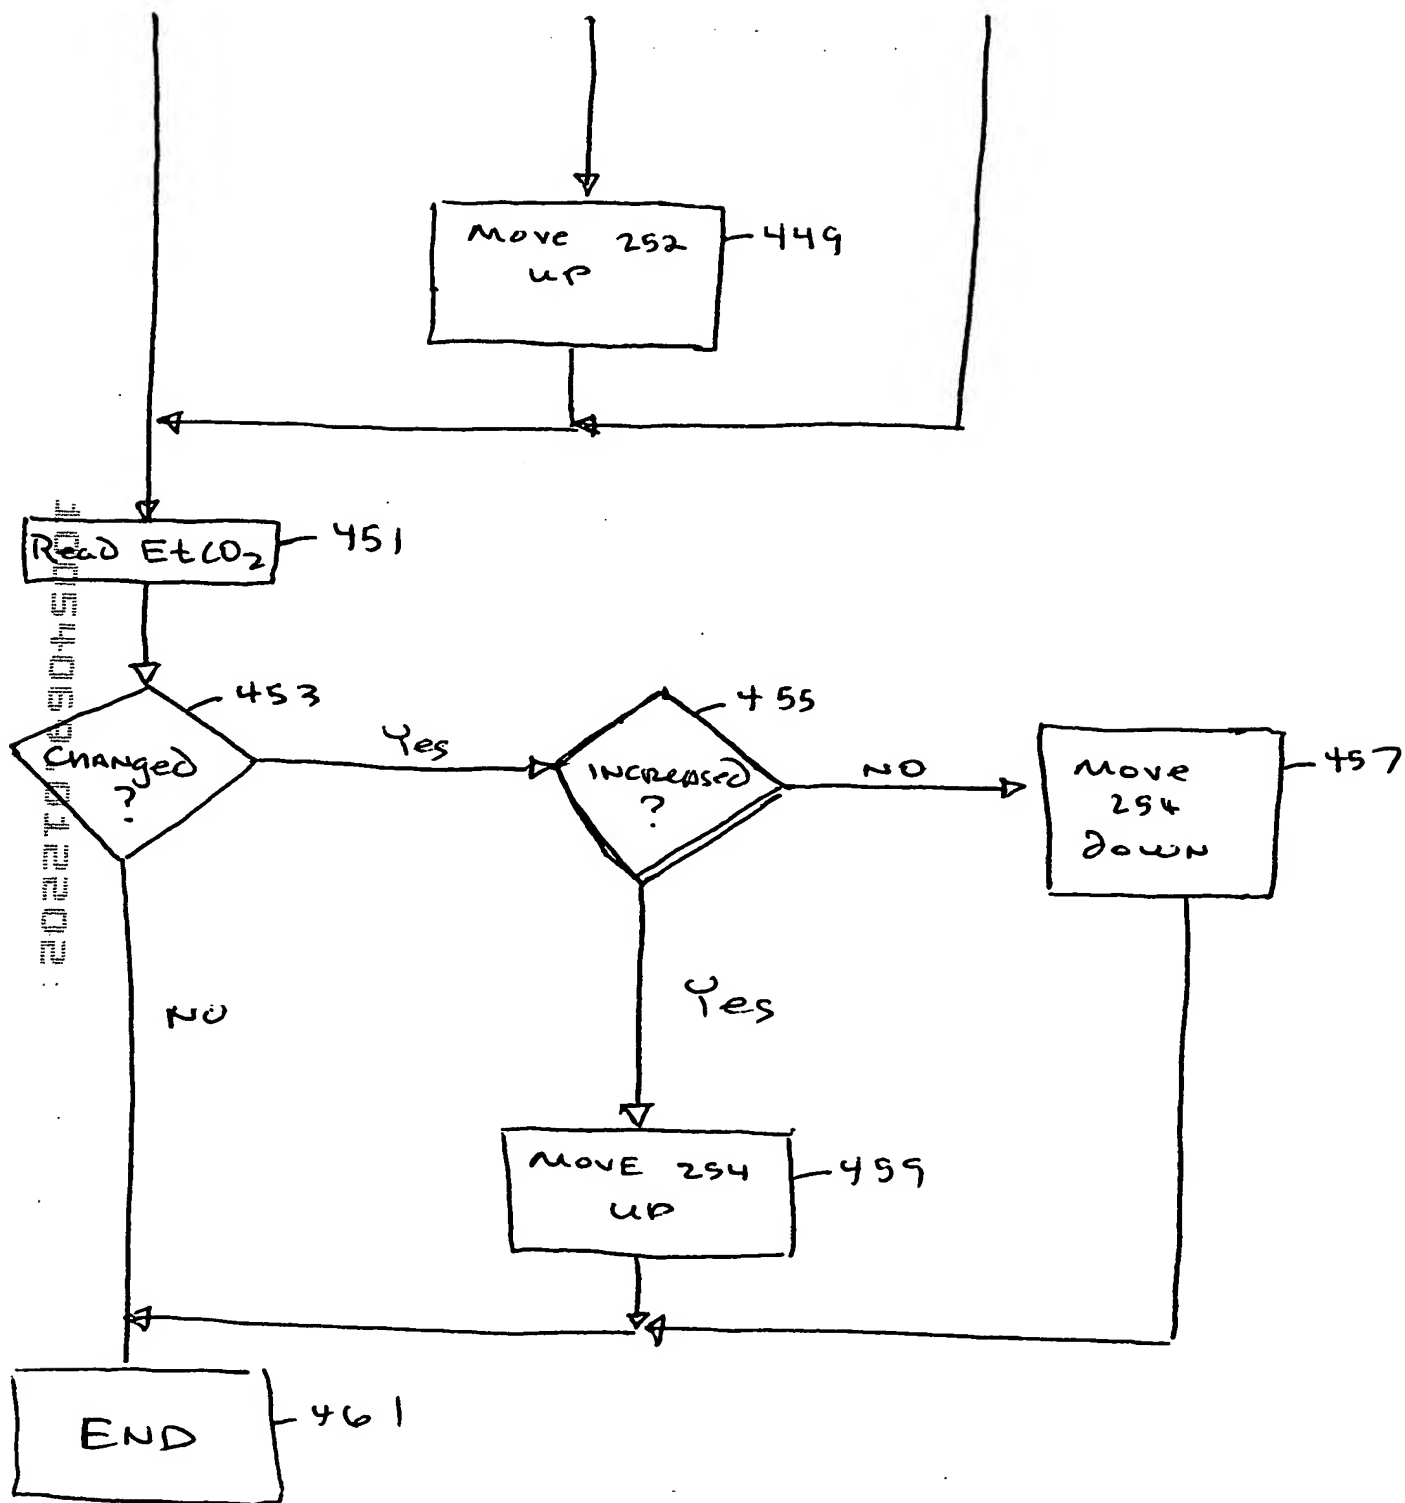


Fig. 15




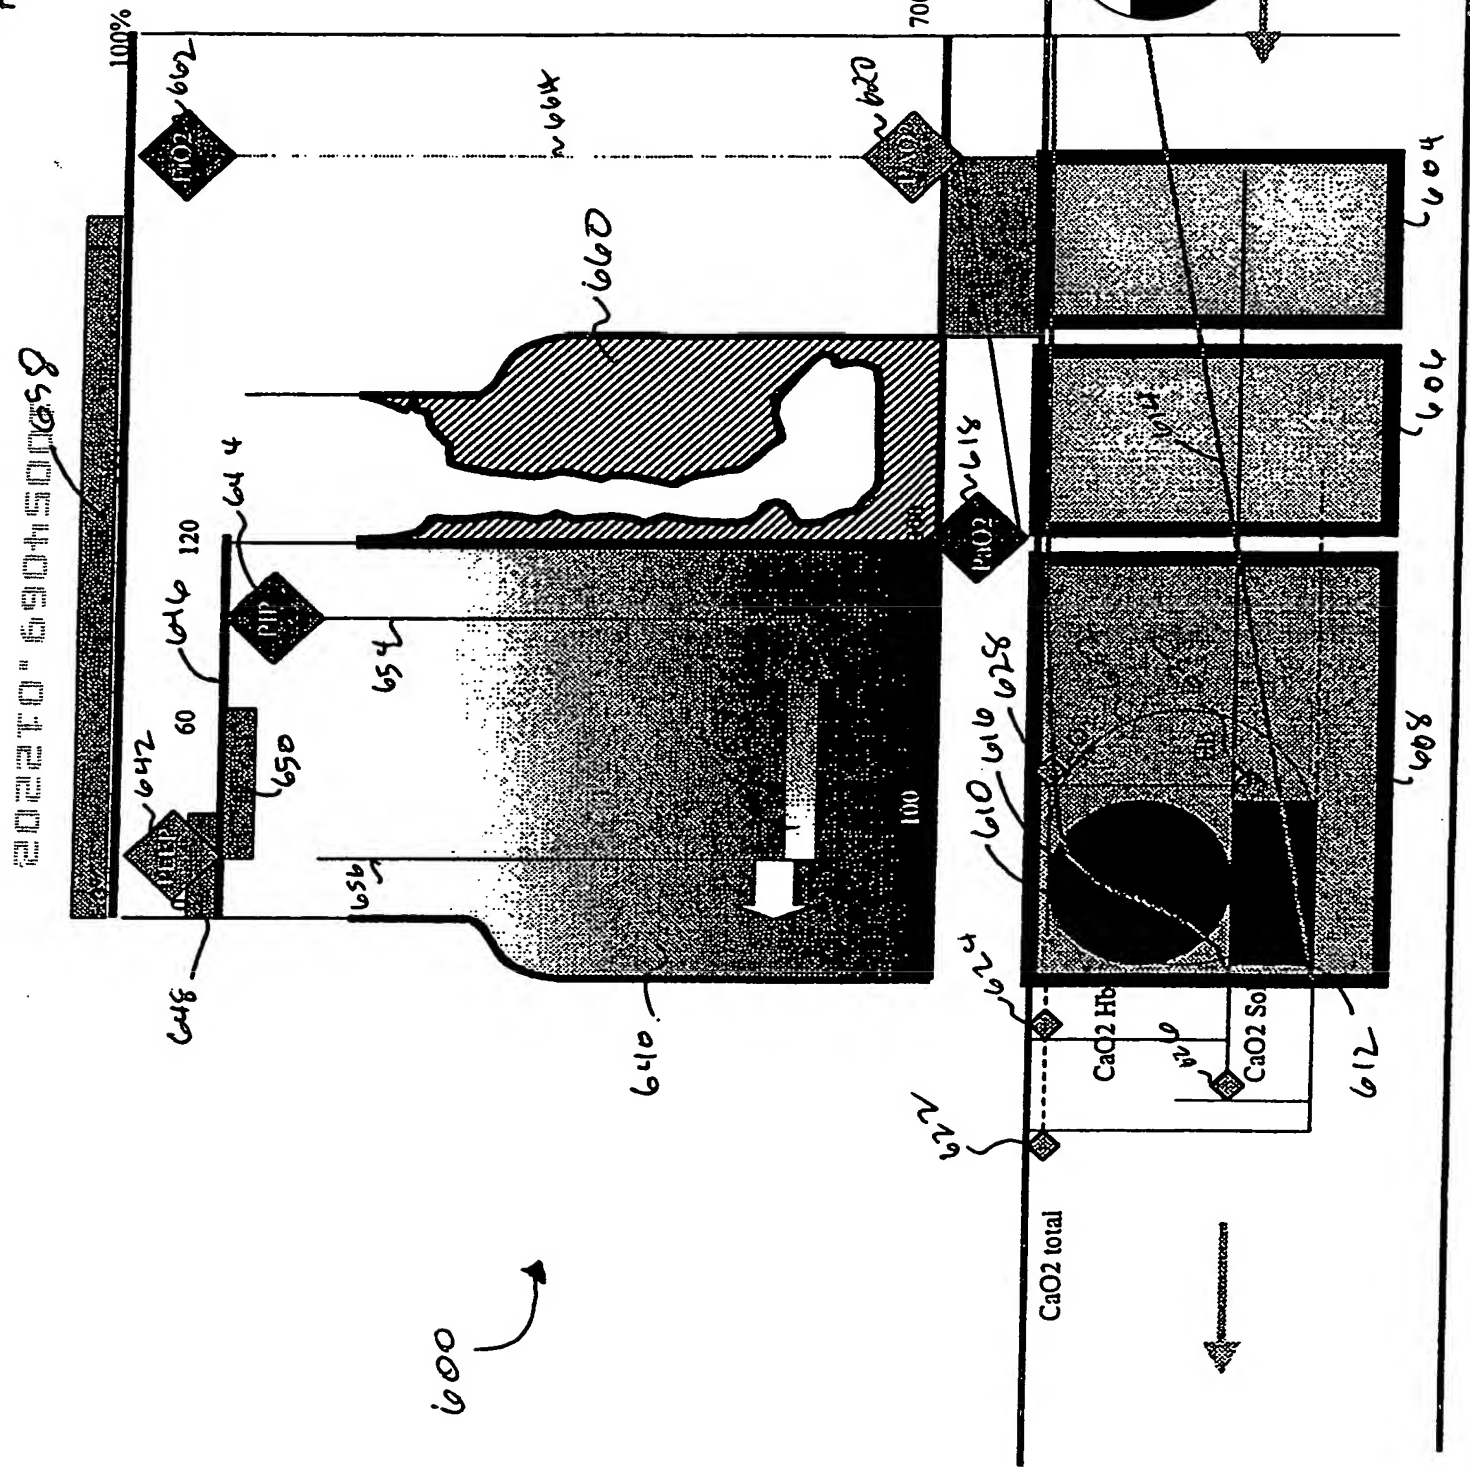


Fig. 16

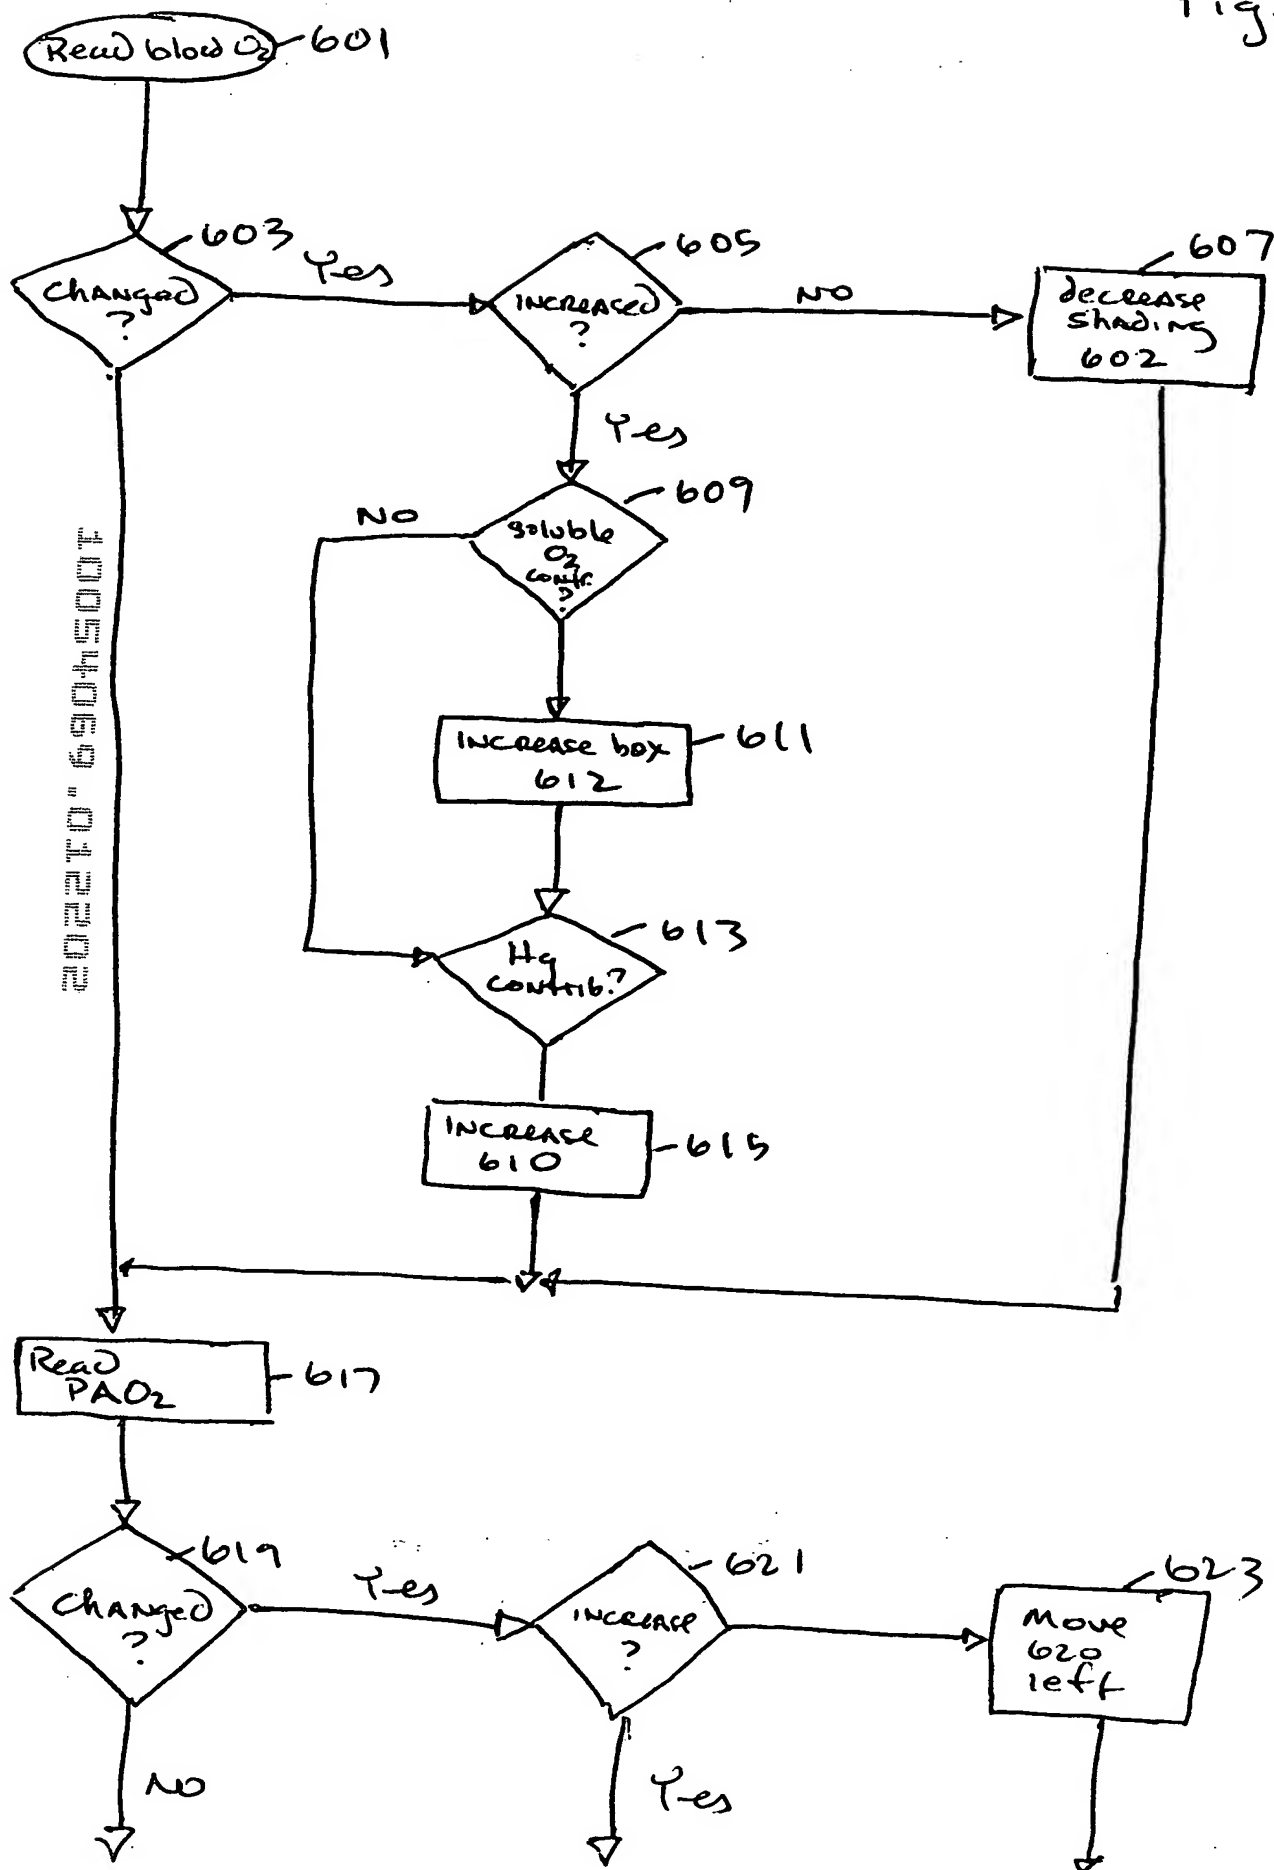

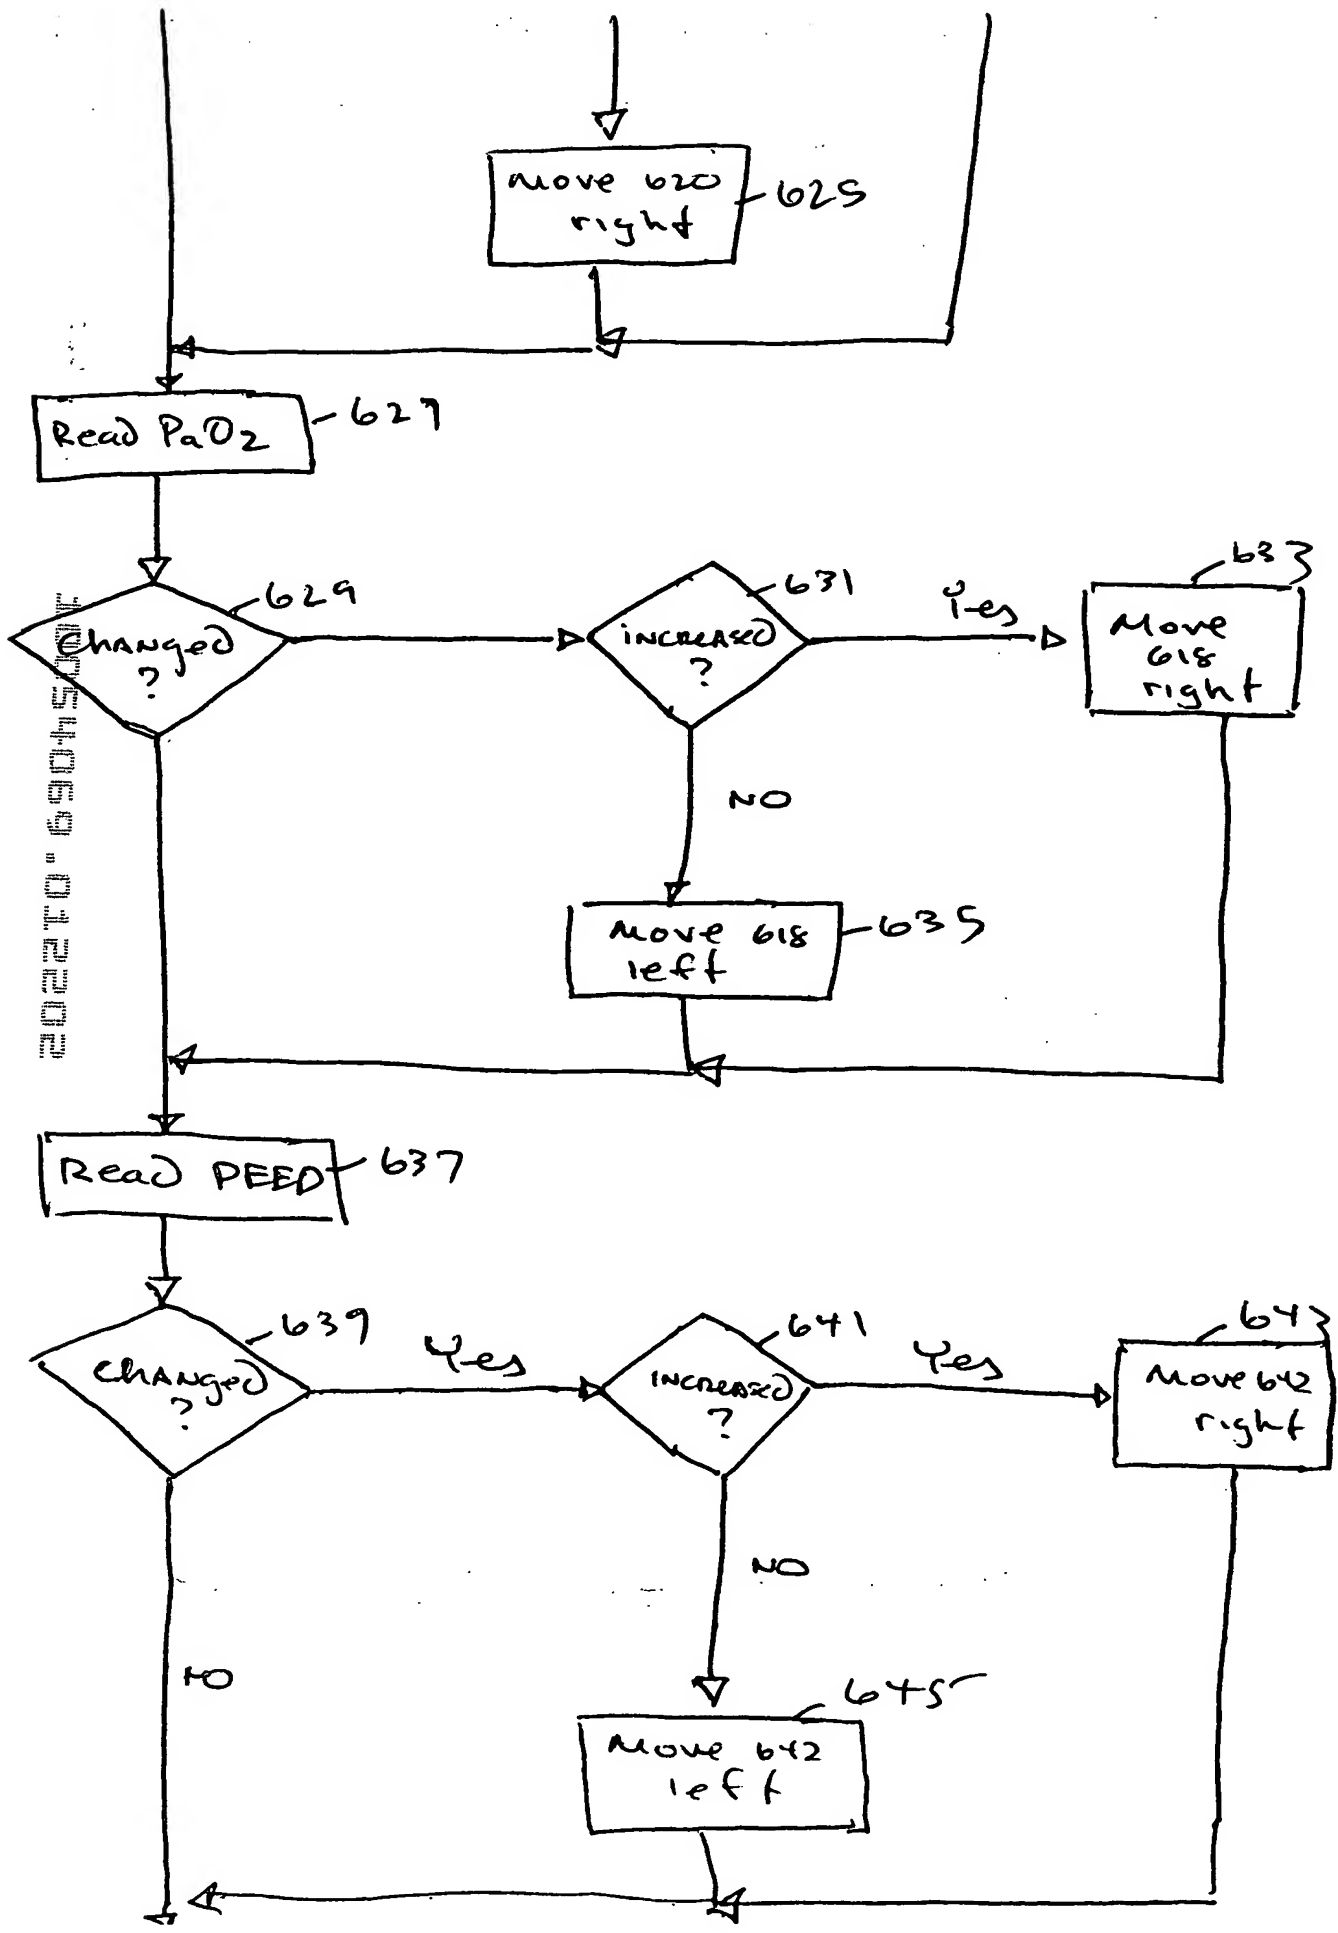

29/32

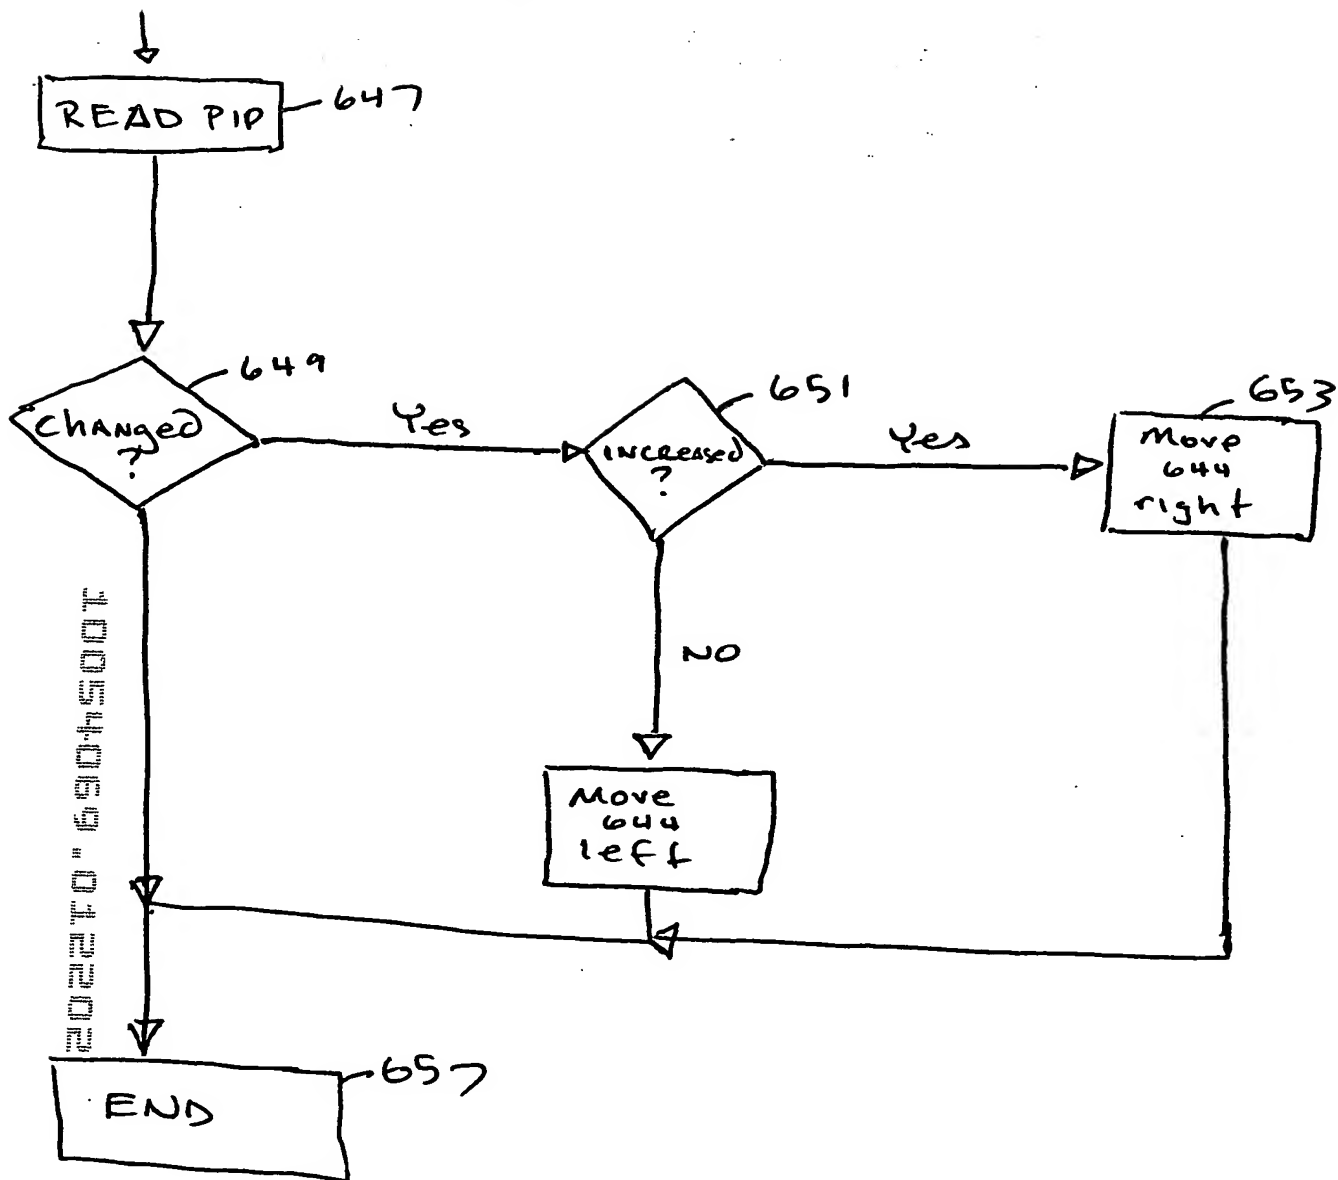

202210169045001

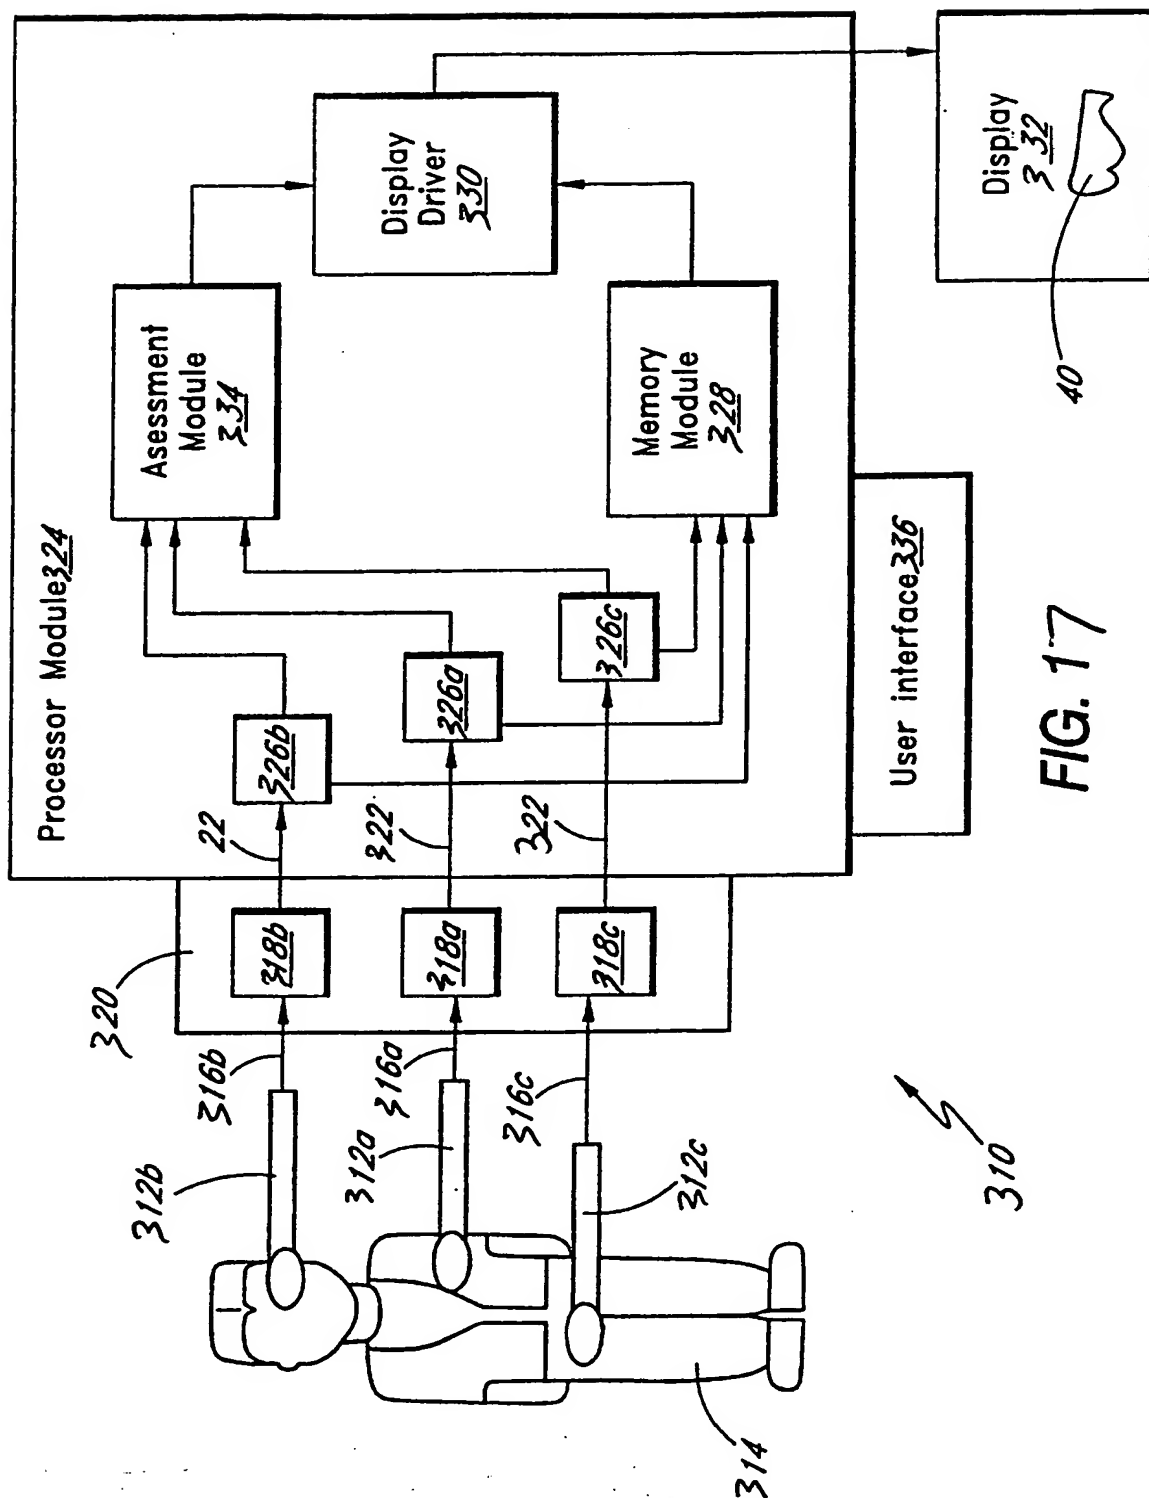


FIG. 17

453022T0 6904500T

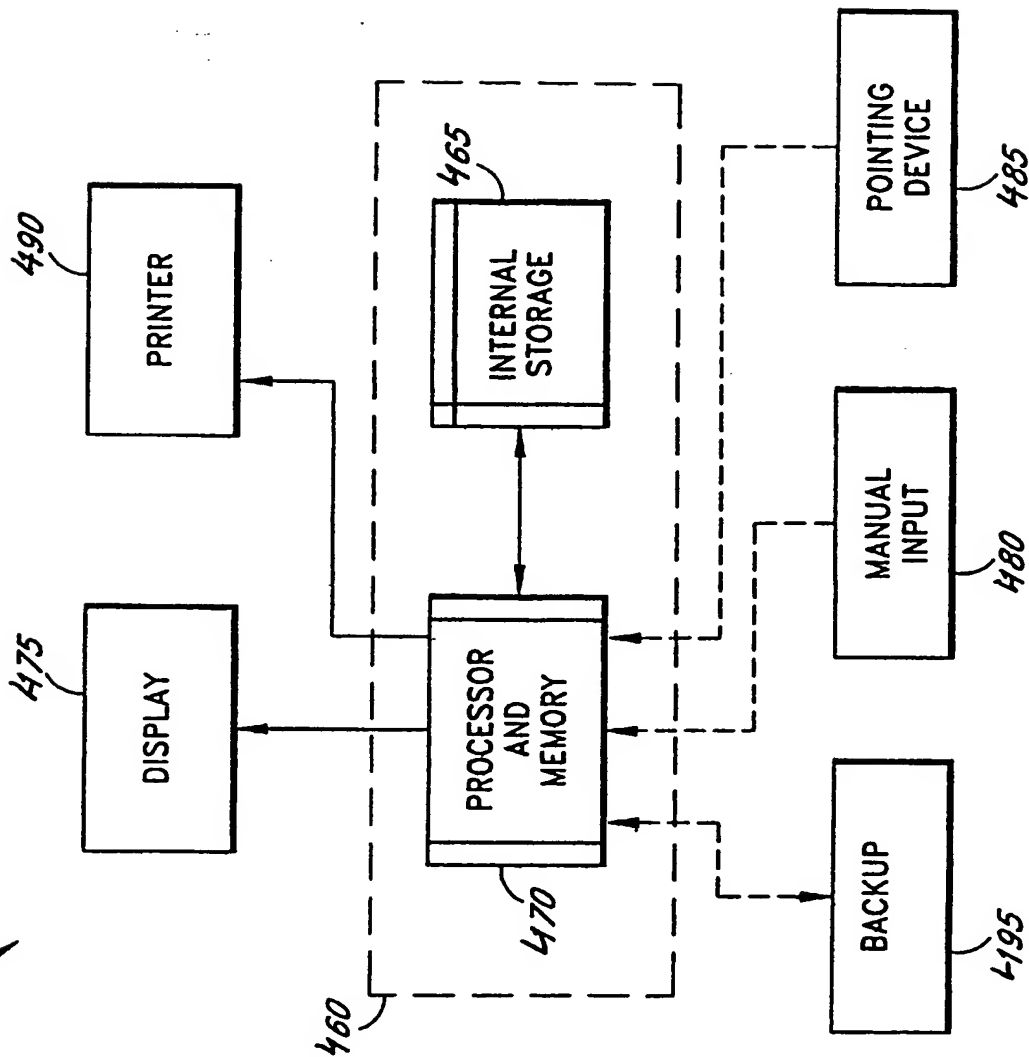


FIG. / 8

